



## **Certification Report**

### **Certified Reference Materials**

**BAM-M383d**

**Pure Copper**

**September 2021**

Coordinator: Dr. Sebastian Recknagel  
Bundesanstalt für Materialforschung und -prüfung (BAM)  
Division 1.6 „Inorganic Reference Materials“  
Richard-Willstätter-Str. 11  
12489 Berlin  
Phone: +49/30/8104 1111  
Fax.: +49/30/8104 71111  
Email: [sebastian.recknagel@bam.de](mailto:sebastian.recknagel@bam.de)

## Summary

This report describes preparation, analysis, and certification of the copper reference material BAM-M383d.

The certified reference material (CRM) is available in the form of discs (ca. 40 mm diameter and 30 mm height). It is intended for establishing and checking the calibration of spark optical emission spectrometers for the analysis of samples of similar materials. It is also suitable for wet chemical analysis.

The following mass fractions and uncertainties have been certified:

Element	Mass fraction <sup>1)</sup> in mg/kg	Uncertainty <sup>2)</sup> in mg/kg
Ag	10.2	0.3
Al	< 1.0	
As	1.20	0.11
Bi	0.82	0.07
Cd	0.62	0.05
Co	1.30	0.06
Cr	0.77	0.12
Fe	22.4	0.9
Mg	1.7	0.2
Mn	0.97	0.09
Ni	4.7	0.4
P	< 1.0	
Pb	7.8	1.0
S	3.5	0.6
Sb	1.8	0.2
Sn	3.8	0.4
Te	0.47	0.05
Ti	1.2	0.3
Zn	1.08	0.14
Zr	< 1.0	

<sup>1)</sup> Unweighted mean value of the means of accepted sets of data (consisting of at least 4 but usually 6 single results), each set being obtained by a different laboratory and/or a different method of measurement.

<sup>2)</sup> Estimated expanded uncertainty  $U$  with a coverage factor of  $k = 2$ , corresponding to a level of confidence of approx. 95 %, as defined in the Guide to the expression of uncertainty in measurement, (GUM, ISO/IEC Guide 98-3:2008).

The certified values are based on the results of 11 laboratories which participated in the certification interlaboratory comparison. The mass fraction of Se is given for information.

## Content

	<b>Page</b>
List of abbreviations .....	5
1. Introduction.....	6
2. Companies/laboratories involved .....	6
3. Candidate material .....	7
4. Homogeneity testing.....	7
5. Characterisation study.....	8
5.1 Analytical procedures .....	8
5.2 Analytical results and statistical evaluation.....	9
6. Instructions for users and stability statement.....	40
7. Metrological Traceability.....	41
8. References .....	41
9. Information on and purchase of the CRM.....	41
Annex 2: Calculation of uncertainty contribution of potential inhomogeneity (length) .....	42
Annex 2: Calculation of uncertainty contribution of potential inhomogeneity (area) .....	54

## List of abbreviations

(if not explained elsewhere)

CRM	certified reference material
ETAAS	electrothermal atomic absorption spectrometry
ICP-OES	inductively coupled plasma optical emission spectrometry
ICP-MS	inductively coupled plasma mass spectrometry
GD-MS	glow discharge mass spectrometry
SOES	spark optical emission spectrometry
$M$	mean value
$n$	number of accepted data sets
$s$	standard deviation of an individual data set
$s_M$	standard deviation of laboratory means
$s_{rel}$	relative standard deviation
$\bar{s}_i$	square root of mean of variances of data sets under repeatability conditions
$M_i$	single result
I	ICP-OES (Tables 2 – 22)
IMS	ICP-MS (Tables 2 – 22)
EA	ETAAS (Tables 2 – 22)
V	Combustion/infrared absorption (Tables 2 – 22)
GD	GD-MS (Tables 2 – 22)

## 1. Introduction

In the metal-producing and metal-processing industry mainly spark optical emission spectrometry (SOES) and X-ray fluorescence spectrometry (XRF) are used for reception inspection of raw materials, e.g. scrap, for quality control of end products and production control. These time-saving analytical techniques require suitable reference materials for calibration and recalibration.

The certified reference material BAM-M383d is based on pure copper. It replaces the out of stock CRMs BAM-M383/BAM-M383a-c. Certification of BAM-M383d was carried out in cooperation with the working group „Copper“ of the Committee of Chemists within the Society of Metallurgists und Miners (GDMB). The needs were defined by this working group, since the members are potential users of the prepared CRM. Participating laboratories were recruited from this group. Since all of them are highly experienced with copper analysis and had participated in earlier inter-laboratory comparisons, there was no preceding round for qualification necessary.

Certification of reference material BAM-M383d was carried out on the basis of ISO 17034 [1] and the relevant ISO-Guides [2, 3].

## 2. Companies/laboratories involved

### Manufacturing of the material

- Wieland-Werke AG, Vöhringen, Germany

### Test for homogeneity

- Bundesanstalt für Materialforschung und -prüfung (BAM), Berlin, Germany
- Participating laboratories

### Participants in the certification inter-laboratory comparison

- Alfred H Knight International, Prescot, Knowsley, United Kingdom
- Aurubis AG, Hamburg, Germany
- Bundesanstalt für Materialforschung und -prüfung (BAM), Berlin, Germany
- Diehl Metall Stiftung & Co KG, Röthenbach, Germany
- Forschungsinstitut Edelmetalle + Metallchemie, Schwäbisch Gmünd, Germany
- Heimerle + Meule GmbH, Pforzheim, Germany
- Inspectorate International Limited, Witham, United Kingdom
- Institut Glörfeld, Willich, Germany
- KM Europa Metal AG, Osnabrück, Germany
- KME Mansfeld GmbH, Hettstedt, Germany
- Łukasiewicz Research Network – Institute of Non-Ferrous Metals, Gliwice, Poland
- Montanwerke Brixlegg, Brixlegg, Austria

### Statistical evaluation of the data

- Bundesanstalt für Materialforschung und -prüfung (BAM), Berlin, Germany

### 3. Candidate material

The candidate material foreseen for CRM BAM-M383d was cast by Wieland-Werke AG, Vöhringen starting with pure copper (Aurubis AG, Hamburg) which was doped with the desired impurities. Starting from the melt a total of 9 billets were cast. Subsequently, the billets were halved and pressed into 18 rods (length: ca. 6000 mm). These rods again were halved and in total 24 rods with a length of 3 m and a diameter of 40 mm were delivered to BAM and then cut into 72 segments of approx. 960 mm length, see Fig. 1. Discs taken between these 1 m rods were taken for analysis. Only discs obtained from Rods 1-6 were used as CRM BAM-M383d

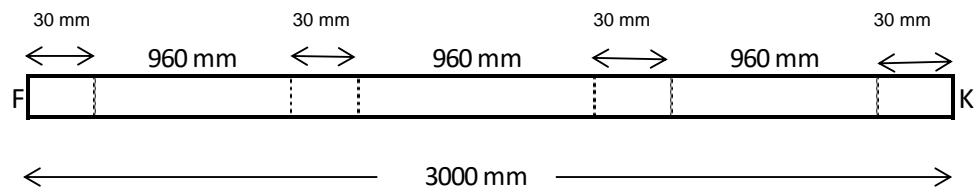


Fig. 1: Cutting plan of pure copper reference material BAM-M383d

About 1700 discs of BAM-M383d with a diameter of approx. 40 mm and 30 mm height were obtained from the total batch.

### 4. Homogeneity testing

BAM-M383d was produced together BAM-M384c. The contents of the impurities in BAM-M383d are quite low. In case of the spark emission spectrometer of BAM, the contents for most of the elements were too low to be determined. Therefore, data from the homogeneity test of BAM-M384c was used instead or an inhomogeneity contribution to the total uncertainty was estimated based on experience with other copper-CRMs (As, Cr, P, Se, Sn, Ti) which were produced in the same way as BAM-M383d. This procedure was already performed when BAM-M383 was certified in 2006. Inhomogeneity contributions related to axial inhomogeneity lay between 0.3 and 3 % rel. Inhomogeneity contributions related to radial inhomogeneity lay between 0.3 and 4 % rel. (see Figure 2). For Ni data from the accompanying spark emission round robin test was used to calculate the inhomogeneity contribution to the total uncertainty. the number of sparks in this round robin was nine (outer circle: 4 sparks, inner circle: 4 sparks; centre: 1 spark). To calculate the necessary data an unbalanced ANOVA was carried out considering that the number of single measurements is different for the centre, the inner and the outer circle. For technical reasons, at  $r_0$  (centre) only one measurement is possible. An ANOVA requires a minimum of two measurements per factor value. Thus, the value for  $r_0$  should be replaced by a dummy. This dummy is defined as follows:

The two values replacing the one measured have a mean equal to the value measured, and a standard deviation equal to the average within-variation. This resembles the situation where one could take two independent measurements at the same place, with values deviating by the average standard deviation (non-destructive testing method). A first guess for the average standard deviation may be calculated from the data for  $r_{in}$  (inner circle) and  $r_{out}$  (outer circle). An inhomogeneity component for the radius of the disc results from these calculations. From all these values, a combined inhomogeneity component is calculated. This component is compared with the within standard deviation calculated from the ANOVA. The higher component is used for the uncertainty calculation.

Annex 1 shows the results of the calculations for axial homogeneity for BAM-M384c, Annex 2 the results of the calculations for radial homogeneity for BAM-M384c.

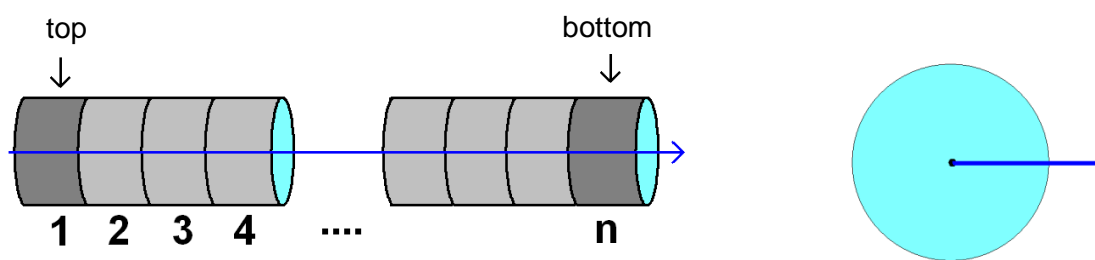


Fig. 2: Axial and radial composition gradient

## 5. Characterisation study

### 5.1 Analytical procedures

Eleven laboratories participated in the certification inter-laboratory comparison. For some elements part of the laboratories used more than one analytical method reporting more than one data set. The laboratories were asked to analyse six subsamples. They were free to choose any suitable analytical method for their determinations. Table 1 shows the analytical methods used by the participating laboratories.

For all analytical procedures where a calibration was necessary this was performed using liquid standard solutions. All participating laboratories were asked to use only standard solutions prepared from pure metals or stoichiometric compounds or traceable commercial calibration solutions.

Table 1: Analytical procedures used by the participating laboratories

Lab-No.	Element	Sample mass	Sample pretreatment	Analytical method
1*	Ag, Al, As, Bi, Cd, Co, Cr, Fe, Mg, Mn, Ni, Pb, Sb, Se, Sn, Te, Ti, Zn, Zr	10 mg	Dissolution with HNO <sub>3</sub>	ICP-MS calibration with commercial solutions
2	Ag, Al, As, Bi, Cd, Co, Cr, Fe, Mg, Mn, Ni, Pb, Sb, Se, Sn, Te, Zn	1 g	Dissolution with HCl/HNO <sub>3</sub> (1 + 1)	ICP-MS, calibration with commercial solution (Spex Certi Prep, traceable to NIST)
	P, Zr	1 g	Dissolution with HCl/HNO <sub>3</sub> (1 + 1)	ICP-OES, matrix matched calibration with commercial solutions (Spex Certi Prep, traceable to NIST)
3*	Ag, Al, As, Bi, Cd, Co, Cr, Fe, Mg, Mn, Ni, P, Pb, S, Sb, Se, Sn, Te, Ti, Zn, Zr	2 g	Dissolution with HCl/HNO <sub>3</sub> /H <sub>2</sub> O (2:1:1)	ICP-OES, matrix matched calibration with commercial solutions (Roth)
4	Ag, Al, As, Bi, Cd, Co, Cr, Fe, Mg, Mn, Ni, P, Pb, S, Sb, Se, Sn, Te, Ti, Zn, Zr	1 g	Dissolution with HNO <sub>3</sub> /HCl	ICP-OES, calibration with commercial standard solutions (Bernd Kraft)
5*	Al, As, P	1 g	Dissolution with HNO <sub>3</sub>	ICP-OES, matrix matched calibration with commercial standard solutions
	Ag, Cd, Co, Cr, Fe, Mg, Mn, Ni, Pb, Sb, Se, Sn, Te, Zn	1 g	Dissolution with HNO <sub>3</sub>	ICP-MS, matrix matched calibration with commercial solutions
6	Ag, As, Cd, Co, Cr, Fe, Mg, Mn, Ni, Pb, S, Sb, Sn, Ti, Zn	1 g	Dissolution with HNO <sub>3</sub>	ICP-OES, matrix matched calibration with commercial standard solutions (Alfa Aesar)
8	Ag, As, Bi, Cd, Co, Cr, Fe, Mg, Mn, Ni, Pb, Sb, Se, Sn, Te, Ti, Zn, Zr	0.5 g	Dissolution with HNO <sub>3</sub> /HCl	ICP-MS, matrix matched calibration with commercial solutions (Bernd Kraft)

\*Laboratory accredited acc. to ISO/IEC 17025



Table 1 (cont.): Analytical procedures used by the participating laboratories

Lab-No.	Element	Sample mass	Sample pretreatment	Analytical method
7	Fe	1 g	Dissolution with HNO <sub>3</sub> /HCl	ICP-OES, matrix matched calibration with standard solutions prepared from pure metals
	Al, As, Bi, Cd, Co, Cr, Mg, Mn, Ni, Pb, Sb, Se, Sn, Te, Zn	1 g	Dissolution with HNO <sub>3</sub> /HCl	ETAAS, matrix matched calibration with standard solutions prepared from pure metals
	Ag	1 g	Dissolution with HNO <sub>3</sub>	ICP-OES, matrix matched calibration with standard solution prepared from pure silver
	S	2 g		Combustion/iodometric titration, calibration with Na <sub>2</sub> S <sub>2</sub> O <sub>3</sub>
9*	As, Bi, Co, Cr, Pb, Sn	1 g	Dissolution with HNO <sub>3</sub>	ETAAS (according to DIN 14935), matrix matched calibration with commercial standard solutions (Merck)
9*	S	1 g		Combustion/IR, calibration with K <sub>2</sub> SO <sub>4</sub>
9	Ag, Al, As, Bi, Cd, Co, Cr, Fe, Mg, Mn, Ni, P, Pb, S, Sb, Se, Si, Sn, Te, Ti, Zn, Zr			GDMS, calibration with ERM-EB383, ERM-EB384, BAM-M384b, BAM-M385a, ERM-EB386, ERM-EB074a and ERM-EB075a
10	As, Cd, Co, Cr, Fe, Mn, Ni, P, Sn, Ti	1 g	Dissolution with HNO <sub>3</sub> /HF/H <sub>3</sub> BO <sub>3</sub>	ICP-OES, matrix matched calibration with commercial mono-element solution (Merck Certipur)
11	Ag, Al, As, Cd, Co, Cr, Fe, Mg, Mn, Ni, P, Se, Sn, Ti, Zr	1 g	Dissolution with HNO <sub>3</sub>	ICP-OES, matrix matched calibration with commercial mono-element solution (Roth)
12	Ag, Al, As, Bi, Cd, Co, Cr, Fe, Mg, Mn, Ni, P, Pb, S, Sb, Se, Sn, Te, Ti, Zn, Zr	0.5 g	Dissolution with HNO <sub>3</sub> /HF	ICP-MS, matrix matched calibration with commercial mono-element solutions (Merck)
13*	Ag, Al, As, Bi, Cd, Co, Cr, Fe, Mg, Mn, Ni, Pb, Sb, Se, Si, Sn, Te, Ti, Zn, Zr	1 g	Dissolution with HNO <sub>3</sub> /HF	ICP-MS, matrix matched calibration with commercial mono-element solutions (Merck, Perkin Elmer)
	Ag, Al, As, Bi, Cd, Co, Cr, Fe, Ni, P, Pb, S, Sb, Se, Si, Sn, Te, Zn	1.5 g	Dissolution with HNO <sub>3</sub> /HF	ICP-OES (1), matrix matched calibration with commercial mono-element solution (Merck, Perkin Elmer, VWR)
	Ag, Cd, Co, Fe, Mg, Mn, Ni, Pb, Sb, Sn, Ti	1.5 g	Dissolution with HNO <sub>3</sub> /HF	ICP-OES (2), matrix matched calibration with commercial multi-element solution (Merck)

\*Laboratory accredited acc. to ISO/IEC 17025

## 5.2 Analytical results and statistical evaluation

The analytical results of the certification inter-laboratory comparison are listed in Tables 2 to 22. These tables show the single results ( $M_i$ ) of each laboratory, the respective laboratories' mean values ( $M$ ), absolute and relative intra-laboratory standard deviation ( $s$  and  $s_{rel}$ , respectively), the standard deviation of laboratory means ( $s_M$ ), and in addition the square root of mean of variances of data sets under repeatability conditions ( $\overline{s}_i$ ), where  $n$  is the number of accepted data sets. The continuous line marks the certified value (mean of the laboratories' means), the broken lines mark the standard deviation, calculated from the laboratories' means.

In the related figures for each laboratory its mean value and single standard deviation is given. Outliers which have been excluded after discussion with the respective laboratories are highlighted in yellow.

Table 2: Results for Ag in BAM-M383d

Lab./Meth.	11/I	6/I	3/I	4/I	13/I-1	1/IMS	5/IMS	7/I	2/IMS	12/IMS	8/IMS	13/I-2	13/IMS	9/GD		
$M_i$ [mg/kg]	8.89	9.48	10.00	9.8	9.72	9.94	10.1	9.99	10.33	10.52	10.50	10.8	10.5	10.7		$n$
	8.83	9.66	9.79	9.7	9.89	9.83	10.1	9.92	10.24	10.45	10.40	10.8	10.5	10.5		13
	8.96	9.10	9.81	10.0	10.07	9.88	10.1	10.10	10.35	10.08	8.93	10.5	10.5	10.5		
	8.67	9.61	9.80	9.7	10.04	10.30	10.0	10.08	10.53	10.67	12.10	10.6	10.5	10.6		
	8.89	9.30	9.64	9.8	10.13	10.15	10.1	10.33	10.43	10.59		10.2	10.6	10.5		
	8.83	9.52	9.84	9.9	10.04	10.05	10.0	10.16	10.24	10.50		10.1	10.6	10.5		
														10.6		
														10.7		
$M$ [mg/kg]	8.8	9.4	9.8	9.8	10.0	10.0	10.1	10.1	10.4	10.5	10.5	10.5	10.5	10.6		10.2
$s$ [mg/kg]	0.1	0.2	0.1	0.1	0.2	0.2	0.0	0.1	0.1	0.2	1.3	0.3	0.1	0.1	$s_M$ [mg/kg]	0.35
$s_{rel}$	0.011	0.022	0.012	0.012	0.015	0.018	0.003	0.014	0.011	0.019	0.124	0.028	0.005	0.005	$\bar{s}_i$ [mg/kg]	0.39
																0.035

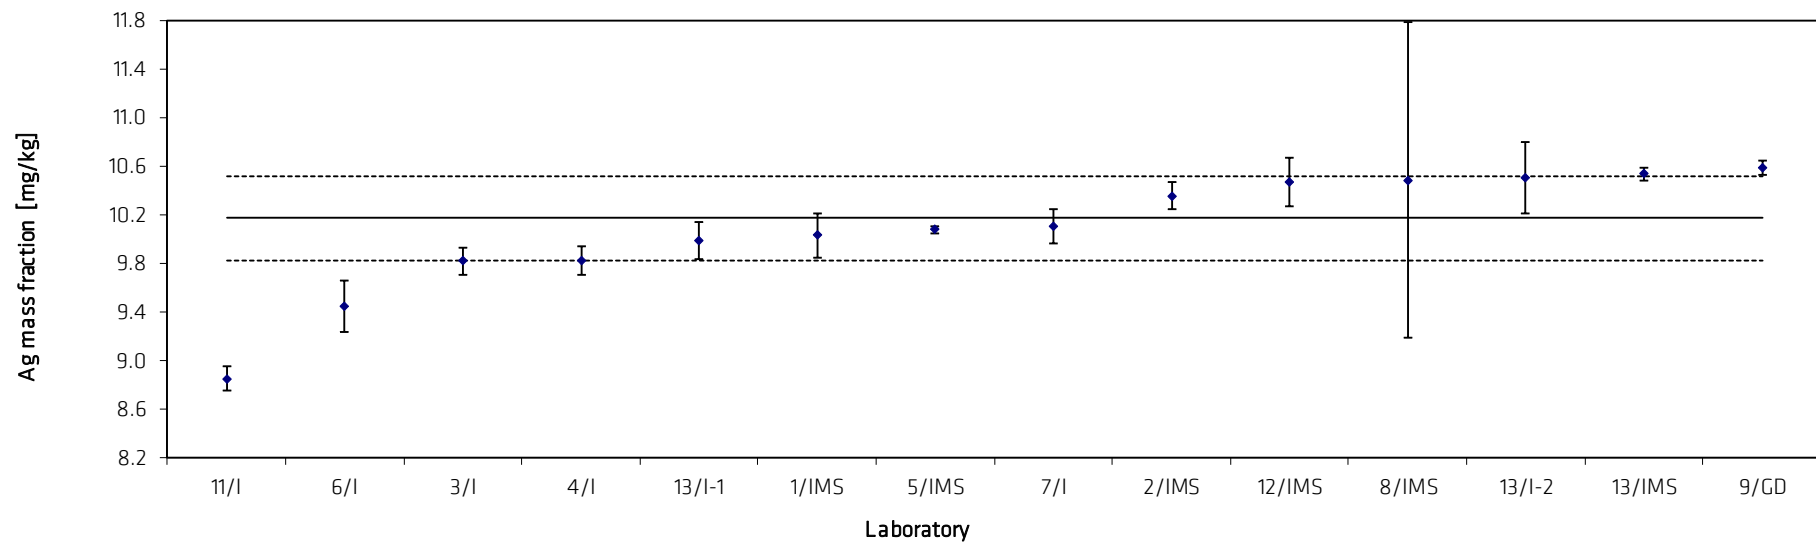


Table 3: Results for Al in BAM-M383d

Lab./Meth.	9/GD	13/I-1	7/EA	11/I	1/IMS	5/I	12/IMS	13/IMS	3/I	4/I	2/IMS		
$M_i$ [mg/kg]	0.063	0.620	0.840	1.850	<0.1	<0.5	<0.9	<1	<1	<1	<5		$n$
	0.068	0.550	0.810	3.070	<0.1	<0.5	<0.9	<1	<1	<1	<5		4
	0.069	0.560	0.860	0.360	<0.1	<0.5	<0.9	<1	<1	<1	<5		
	0.068	0.550	0.820	1.120	<0.1	<0.5	<0.9	<1	<1	<1	<5		
	0.093	0.580	0.870	2.430	<0.1	<0.5	<0.9	<1	<1		<5		
	0.073	0.590	0.800	0.370	<0.1	<0.5	<0.9	<1	<1		<5		
	0.071 0.070												
$M$ [mg/kg]	0.072	0.575	0.833	1.533	<0.1	<0.5	<0.9	<1	<1	<1	<5		0.75
$s$ [mg/kg]	0.0	0.0	0.0	1.1								$s_M$ [mg/kg]	0.61
$s_{rel}$	0.1452	0.0476	0.0337	0.7243								$\bar{s}_i$ [mg/kg]	0.34
													0.8073

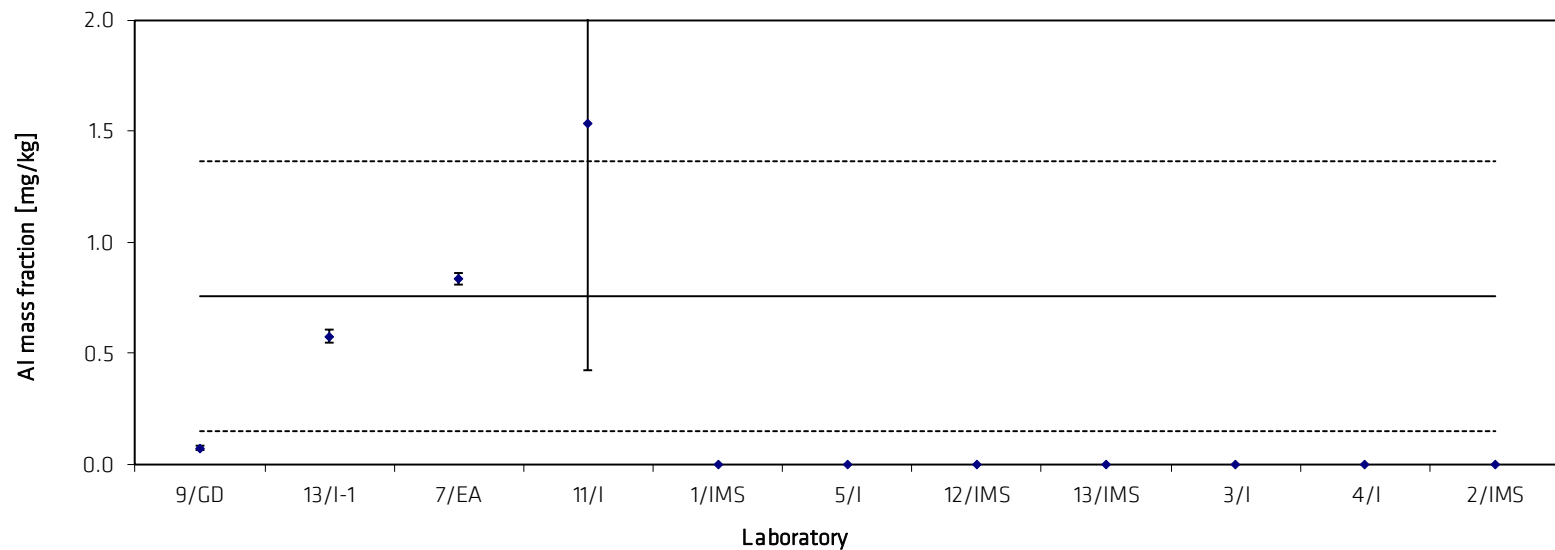


Table 4: Results for As in BAM-M383d

Lab./Meth.	10/I	7/EA	4/I	3/I	12/IMS	13/IMS	8/IMS	1/IMS	9/GD	2/IMS	11/I	5/I	6/I	9/EA		
$M_i$ [mg/kg]	1.0	1.1	1.0	1.14	1.16	1.16	1.44	1.24	1.30	1.38	1.61	1.5	1.30	3.04		$n$ 13
	1.2	1.0	1.1	1.10	1.13	1.14	1.42	1.20	1.26	1.37	1.43	1.2	1.55	3.27		
	1.0	1.0	1.3	1.10	1.08	1.11	0.92	1.26	1.25	1.24	1.27	1.2	1.29	2.94		
	0.8	1.0	1.1	1.12	1.12	1.19	0.83	1.18	1.23	1.35	1.14	1.6	1.76	3.17		
	0.8	1.1	1.0	1.13	1.12	1.13		1.21	1.33	1.36	1.40	1.5	1.71	3.42		
	1.0	1.0	1.0	1.09	1.09	1.13		1.21	1.31	1.24	1.09	1.2	1.72	2.98		
									1.32							
									1.28							
$M$ [mg/kg]	0.97	1.03	1.08	1.11	1.12	1.14	1.15	1.22	1.29	1.32	1.32	1.36	1.56	3.14		1.20
$s$ [mg/kg]	0.1	0.1	0.1	0.0	0.0	0.0	0.3	0.0	0.0	0.1	0.2	0.2	0.2	0.2	$s_M$ [mg/kg]	0.159
$s_{rel}$	0.150	0.049	0.108	0.018	0.027	0.025	0.280	0.024	0.026	0.050	0.147	0.161	0.137	0.059	$\bar{s}_i$ [mg/kg]	0.147
																0.132

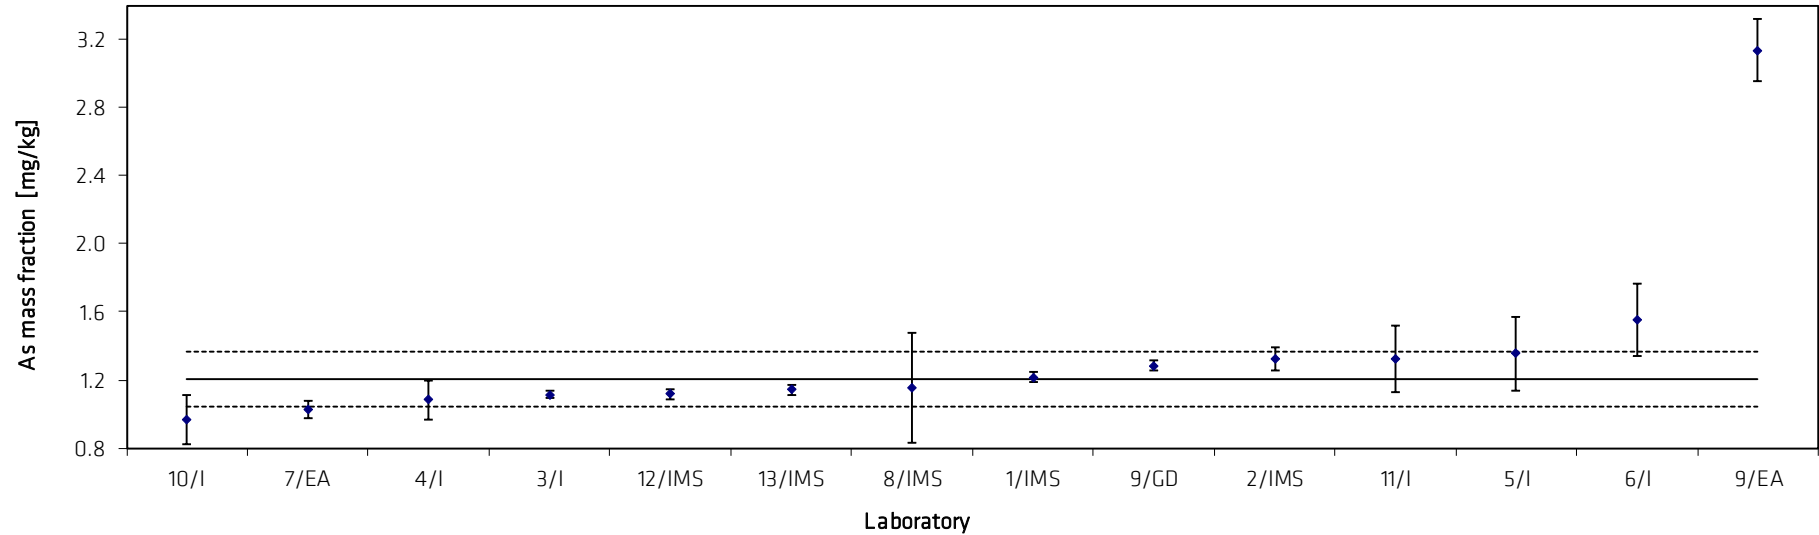


Table 5: Results for Bi in BAM-M383d

Lab./Meth.	12/IMS	1/IMS	2/IMS	9/GD	8/IMS	13/IMS	7/EA	3/I	4/I		
$M_i$ [mg/kg]	0.73	0.76	0.78	0.80	0.85	0.94	0.87	<1	<2		$n$
	0.74	0.77	0.79	0.83	0.82	0.89	0.95	<1	<2		7
	0.71	0.78	0.79	0.78	0.85	0.93	0.90	<1	<2		
	0.74	0.75	0.80	0.83	0.84	0.85	0.98	<1	<2		
	0.73	0.75	0.80	0.78	0.79	0.89	0.85	<1	<2		
	0.71	0.75	0.80	0.80	0.78	0.92	0.92	<1	<2		
				0.79	0.81						
$M$ [mg/kg]	<b>0.73</b>	<b>0.76</b>	<b>0.79</b>	<b>0.80</b>	<b>0.82</b>	<b>0.90</b>	<b>0.91</b>	<b>&lt;1</b>	<b>&lt;2</b>		<b>0.82</b>
$s$ [mg/kg]	0.01	0.01	0.01	0.02	0.03	0.03	0.05			$s_M$ [mg/kg]	0.069
$s_{rel}$	0.0178	0.0166	0.0116	0.0272	0.0372	0.0368	0.0535			$\bar{s}_i$ [mg/kg]	0.024
											0.0843

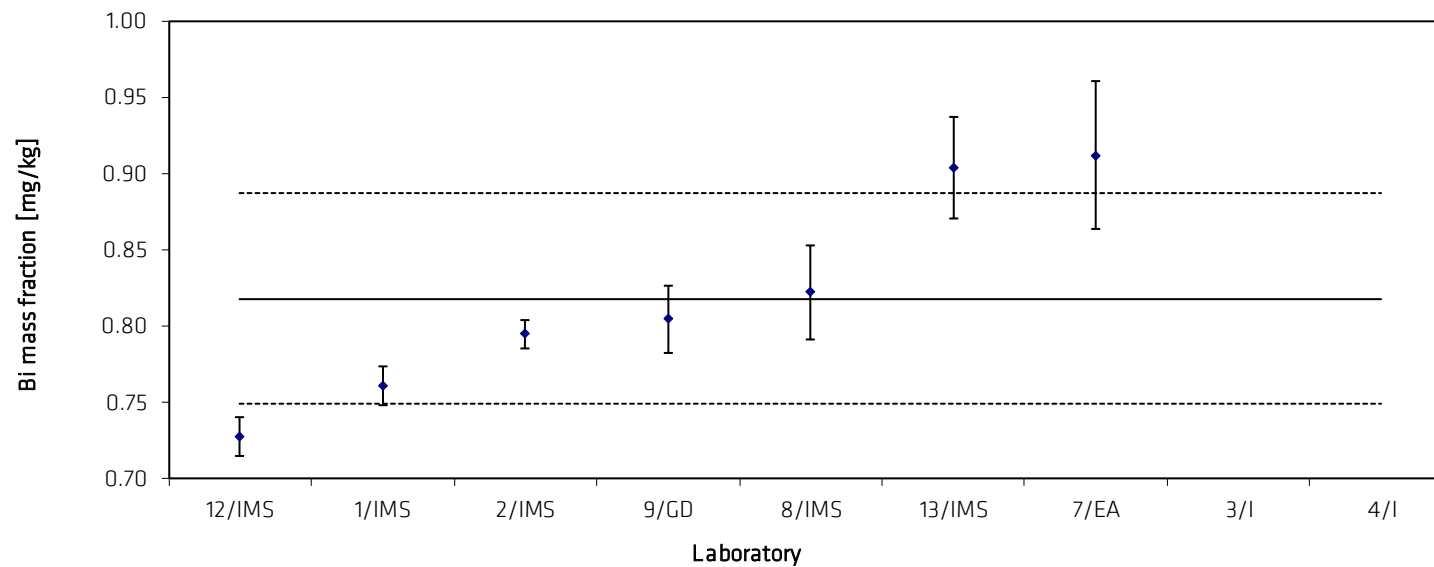


Table 6: Results for Cd in BAM-M383d

Lab./Meth.	4/I	8/IMS	6/I	13/I-1	2/IMS	9/GD	10/I	11/I	5/IMS	12/IMS	13/IMS	1/IMS	9/EA	13/I-2	7/EA	3/I		
$M_i$ [mg/kg]	0.5	0.54	0.61	0.63	0.57	0.62	0.66	0.61	0.62	0.64	0.61	0.65	0.70	0.77	0.90	<1		$n$
	0.5	0.49	0.57	0.59	0.62	0.62	0.65	0.61	0.63	0.64	0.63	0.68	0.68	0.77	0.89	<1		14
	0.5	0.56	0.54	0.62	0.57	0.60	0.61	0.61	0.63	0.61	0.61	0.65	0.72	0.74	0.88	<1		
	0.5	0.51	0.54	0.61	0.64	0.62	0.66	0.67	0.62	0.65	0.72	0.69	0.69	0.75	0.86	<1		
	0.5	0.65	0.56	0.57	0.67	0.63	0.58	0.60	0.62	0.64	0.63	0.69	0.70	0.72	0.89	<1		
	0.5		0.59	0.64	0.63	0.64	0.57	0.63	0.62	0.63	0.62	0.69	0.67	0.73	0.80	<1		
						0.62												
						0.62												
$M$ [mg/kg]	0.50	0.55	0.57	0.61	0.61	0.62	0.62	0.62	0.62	0.63	0.64	0.68	0.69	0.75	0.87	<1		0.62
$s$ [mg/kg]	0.0	0.1	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.0			$s_M$ [mg/kg]
																		0.060
																		$\bar{s}_i$ [mg/kg]
$s_{rel}$	0.0000	0.1128	0.0490	0.0427	0.0642	0.0153	0.0655	0.0412	0.0060	0.0218	0.0656	0.0293	0.0253	0.0277	0.0424			0.030
																		0.0965

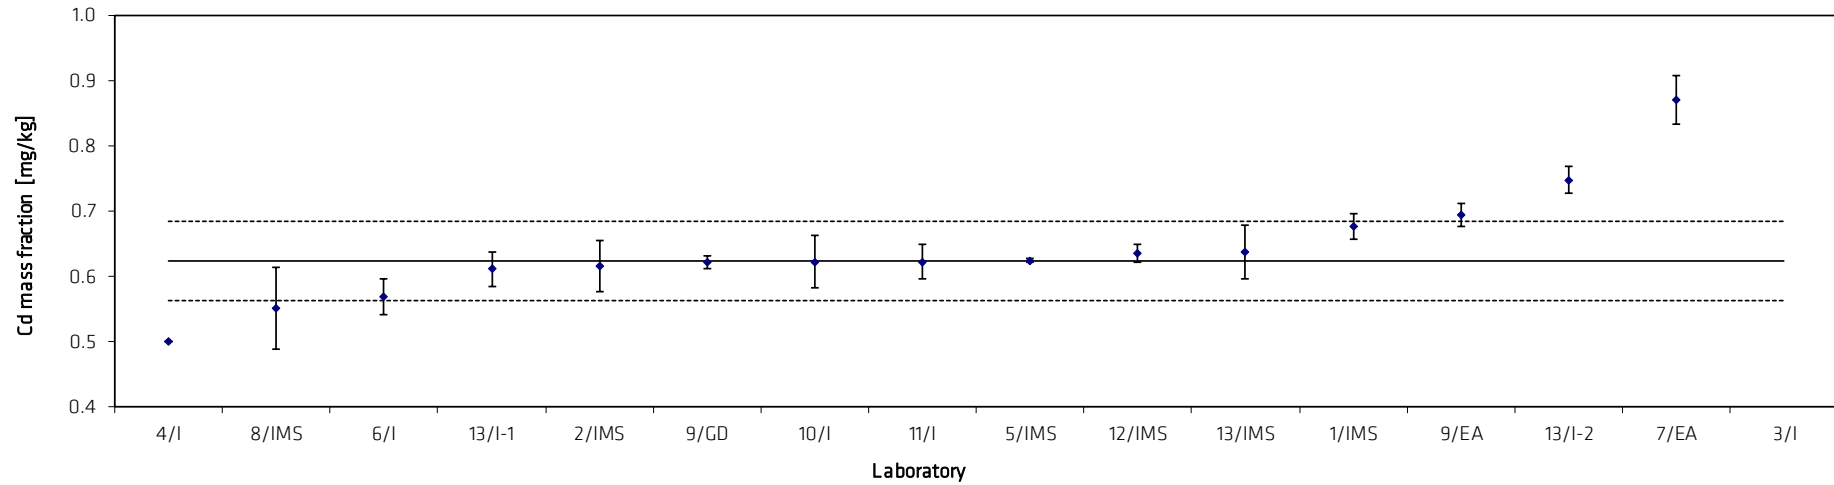


Table 7: Results for Co in BAM-M383d

Lab./Meth.	13/I-1	13/I-2	6/I	2/IMS	5/IMS	3/I	11/I	9/EA	13/IMS	1/IMS	9/GD	12/IMS	8/IMS	10/I	7/EA		
$M_i$ [mg/kg]	1.13	1.20	1.16	1.24	1.27	1.31	1.30	1.33	1.31	1.36	1.36	1.36	1.46	1.49	1.99		$n$ 14
	1.17	1.50	1.13	1.18	1.27	1.29	1.28	1.26	1.34	1.33	1.34	1.32	1.41	1.46	1.90		
	1.07	1.20	1.31	1.21	1.26	1.29	1.32	1.27	1.27	1.36	1.41	1.42	1.42	1.55	1.85		
	1.14	1.20	1.30	1.27	1.27	1.28	1.32	1.28	1.36	1.30	1.36	1.35	1.44	1.46	1.80		
	1.14	1.10	1.12	1.24	1.27	1.27	1.25	1.29	1.32	1.30	1.34	1.36	1.36	1.47	1.94		
	1.22	1.00	1.27	1.21	1.26	1.27	1.26	1.30	1.33	1.30	1.31	1.46	1.34	1.41	1.81		
											1.38	1.34					
$M$ [mg/kg]	1.15	1.20	1.22	1.23	1.27	1.29	1.29	1.29	1.32	1.33	1.35	1.38	1.41	1.47	1.88		1.30
$s$ [mg/kg]	0.0	0.2	0.1	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.1	0.0	0.0	0.1	$s_M$ [mg/kg]	0.088
$s_{rel}$	0.0431	0.1394	0.0723	0.0245	0.0035	0.0118	0.0232	0.0193	0.0232	0.0223	0.0236	0.0374	0.0330	0.0312	0.0400	$\bar{s}_i$ [mg/kg]	0.060
																	0.0675

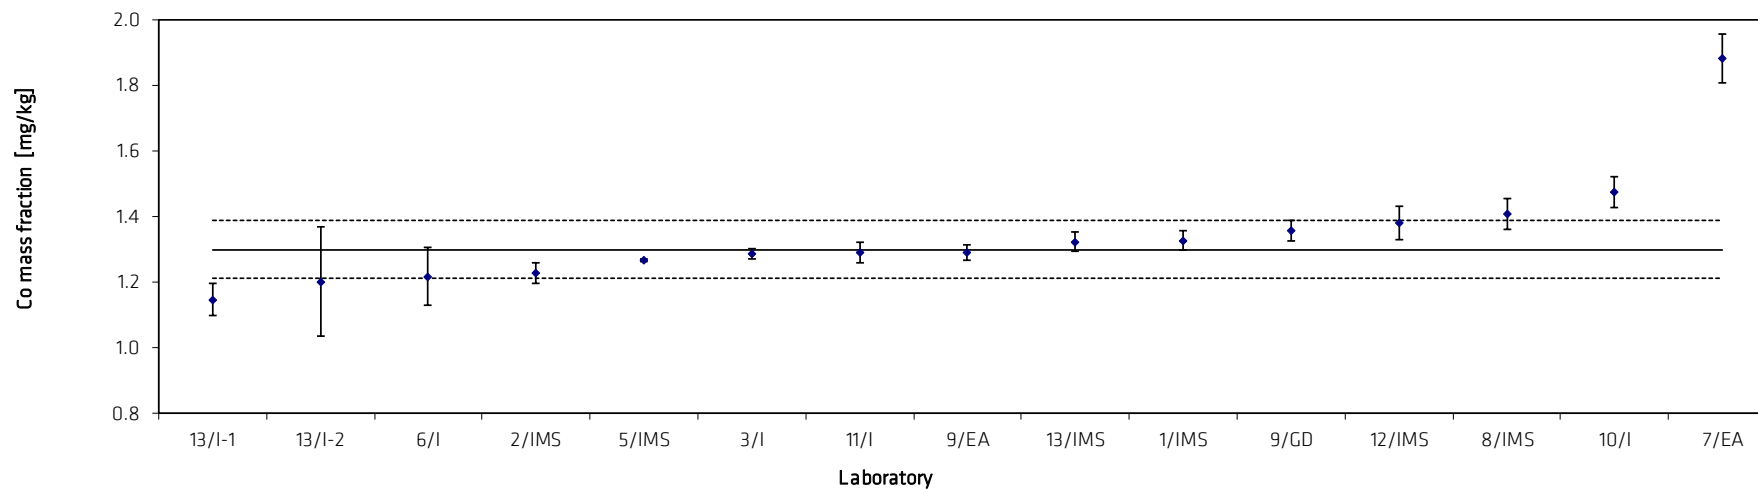


Table 8: Results for Cr in BAM-M383d

Lab./Meth.	11/I	1/IMS	13/IMS	6/I	5/IMS	4/I	10/I	13/I-1	9/GD	9/EA	12/IMS	8/IMS	2/IMS	7/EA	3/I		
$M_i$ [mg/kg]	0.03	0.26	0.50	0.52	0.60	0.5	0.7	0.79	0.77	0.80	0.85	0.95	0.95	1.11	<1		$n$
	0.07	0.16	0.52	0.58	0.67	0.8	0.7	0.72	0.77	0.76	0.85	0.90	0.92	1.22	<1		12
	0.15	0.17	0.41	0.62	0.67	0.8	0.7	0.78	0.76	0.80	0.88	0.83	0.92	1.05	<1		
	0.13	0.50	0.45	0.49	0.65	0.6	0.7	0.71	0.75	0.79	0.86	0.83	1.13	1.15	<1		
	0.30	0.49	0.48	0.50	0.63	0.6	0.8	0.79	0.79	0.96	0.86	0.83	0.82	1.25	<1		
	0.28	0.49	0.54	0.58	0.63	0.6	0.8	0.70	0.79	0.85	0.85		0.92	1.20	<1		
									0.77								
									0.80								
<b><math>M</math> [mg/kg]</b>	<b>0.16</b>	<b>0.35</b>	<b>0.48</b>	<b>0.55</b>	<b>0.64</b>	<b>0.65</b>	<b>0.74</b>	<b>0.75</b>	<b>0.77</b>	<b>0.83</b>	<b>0.86</b>	<b>0.87</b>	<b>0.94</b>	<b>1.16</b>	<b>&lt;1</b>		<b>0.77</b>
$s$ [mg/kg]	0.11	0.17	0.05	0.05	0.03	0.12	0.06	0.04	0.02	0.07	0.01	0.05	0.10	0.07		$s_M$ [mg/kg]	0.183
$s_{rel}$	0.685	0.482	0.099	0.095	0.043	0.188	0.080	0.057	0.021	0.086	0.014	0.063	0.108	0.064		$\bar{s}_i$ [mg/kg]	0.075
																	0.238

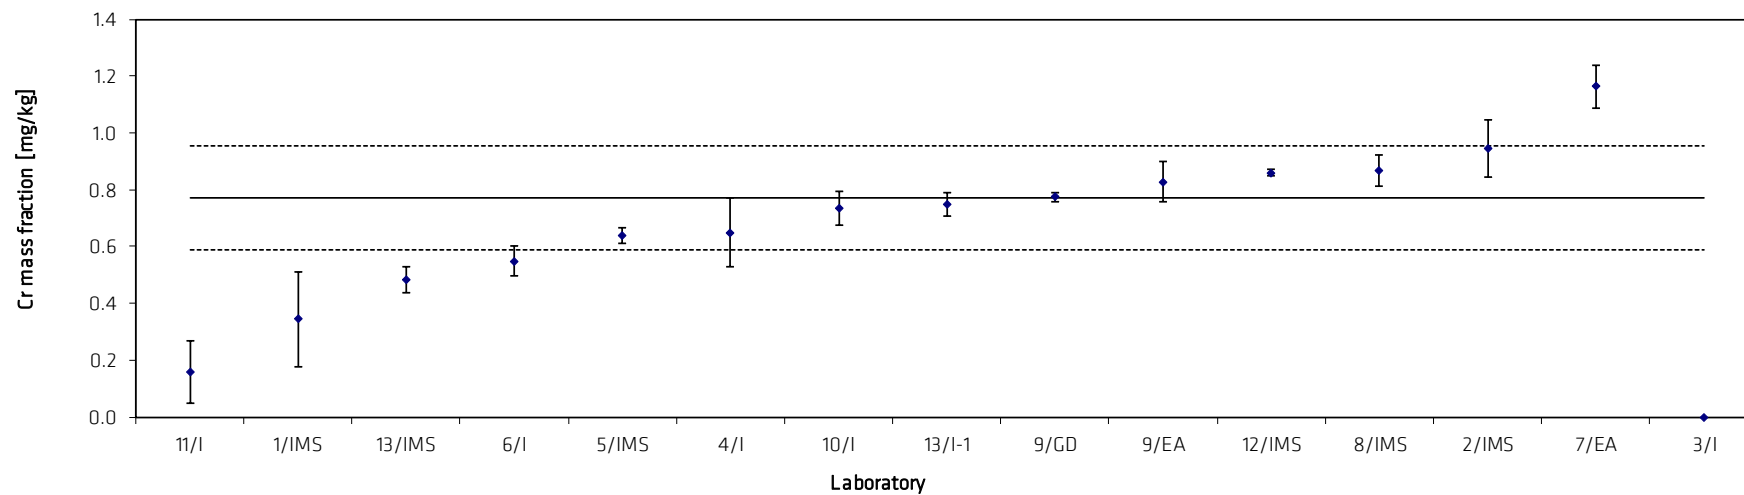




Table 9: Results for Fe in BAM-M383d

Lab./Meth.	11/I	13/IMS	5/IMS	7/I	10/I	6/I	13/I-1	1/IMS	12/IMS	4/I	3/I	2/IMS	13/I-2	9/GD		
$M_i$ [mg/kg]	17.5	20.6	20.9	21.1	21.5	21.7	21.8	20.6	22.8	21	23.6	22.8	24.2	24.0		$n$
	18.1	20.9	21.1	20.9	21.5	21.7	22.1	20.3	22.6	24	22.9	22.9	24.9	23.9		13
	18.0	20.3	20.7	21.0	21.3	22.5	21.9	20.0	22.8	26	23.0	23.3	24.6	25.0		
	18.0	20.9	21.1	21.3	21.5	21.0	22.5	23.7	23.4	22	22.9	23.9	24.5	24.3		
	18.3	20.4	20.9	21.2	21.7	21.2	21.5	23.8	22.7	22	22.8	23.4	24.4	25.1		
	18.2	20.0	20.6	21.0	21.5	21.8	22.1	24.1	22.6	22	22.9	28.4	23.9	24.7		
														24.9		
														24.7		
$M$ [mg/kg]	18.0	20.5	20.9	21.1	21.5	21.6	22.0	22.1	22.8	22.8	23.0	24.1	24.4	24.6		22.4
$s$ [mg/kg]	0.3	0.4	0.2	0.1	0.1	0.5	0.3	2.0	0.3	1.8	0.3	2.1	0.3	0.5	$s_M$ [mg/kg]	1.35
$s_{rel}$	0.0169	0.0173	0.0105	0.0061	0.0060	0.0248	0.0158	0.0896	0.0132	0.0804	0.0119	0.0883	0.0140	0.0190	$\bar{s}_i$ [mg/kg]	1.00
																0.0601

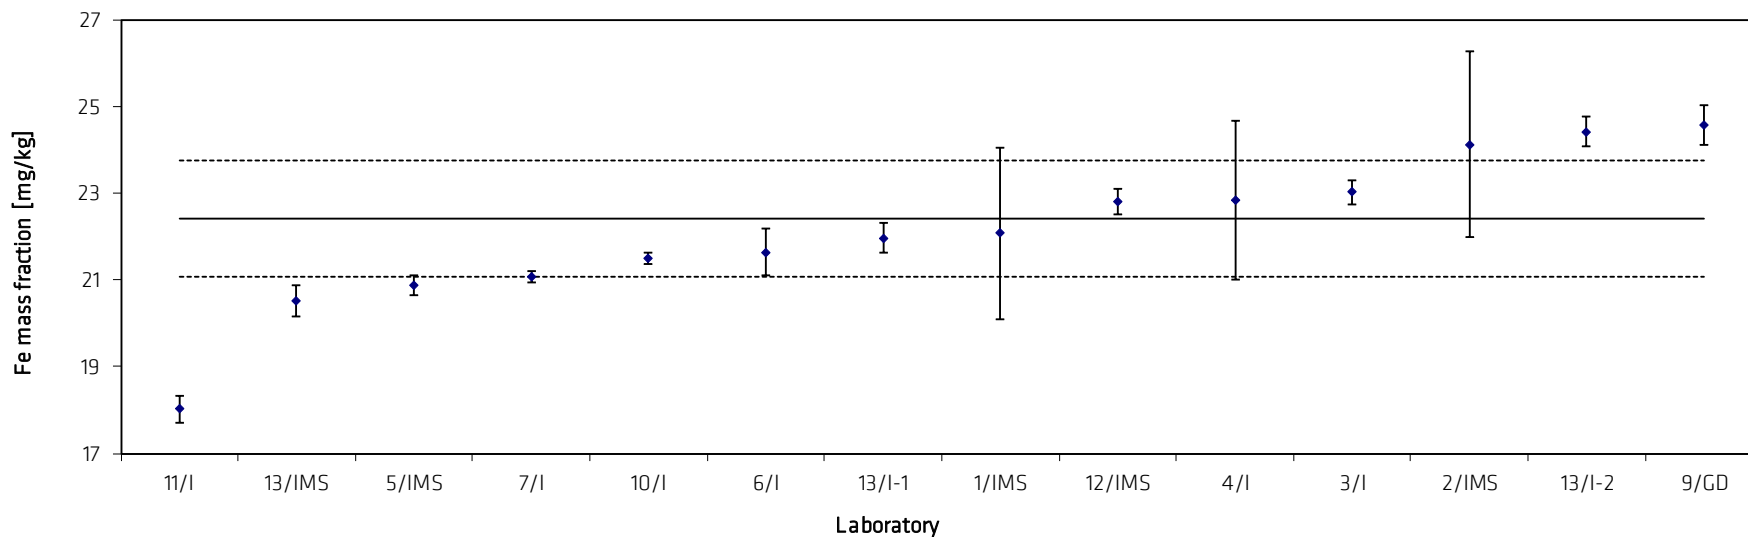


Table 10: Results for Mg in BAM-M383d

Lab./Meth.	11/I	5/IMS	6/I	3/I	4/I	13/IMS	12/IMS	8/IMS	7/EA	13/I-2	9/GD	1/IMS	2/IMS		
$M_i$ [mg/kg]	0.93	1.27	1.53	1.63	1.5	1.6	1.8	1.9	1.9	1.7	2.22	3.77	<5		$n$ 11
	1.11	1.34	1.42	1.57	1.8	1.6	1.8	1.9	1.8	2.4	2.05	4.02	<5		
	0.91	1.36	1.80	1.54	1.9	1.5	1.8	1.9	1.9	1.8	2.01	4.15	<5		
	0.96	1.26	1.36	1.57	1.5	1.8	1.7	1.6	1.8	2.2	1.92	4.12	<5		
	1.42	1.41	1.45	1.57	1.5	1.7	1.8		1.8	2.2	2.22	4.30	<5		
	0.92	1.40	1.60	1.46	1.5	1.6	1.7		1.9	2.0	2.12	4.43	<5		
											2.12				
											2.06				
$M$ [mg/kg]	<b>1.04</b>	<b>1.34</b>	<b>1.53</b>	<b>1.56</b>	<b>1.62</b>	<b>1.63</b>	<b>1.78</b>	<b>1.81</b>	<b>1.85</b>	<b>2.05</b>	<b>2.09</b>	<b>4.13</b>	<5		<b>1.66</b>
$s$ [mg/kg]	0.20	0.06	0.16	0.06	0.18	0.10	0.07	0.12	0.07	0.27	0.10	0.23		$s_M$ [mg/kg]	0.30
$s_{rel}$	0.1916	0.0474	0.1036	0.0365	0.1135	0.0632	0.0391	0.0657	0.0355	0.1300	0.0485	0.0553		$\bar{s}_i$ [mg/kg]	0.14
															0.1829

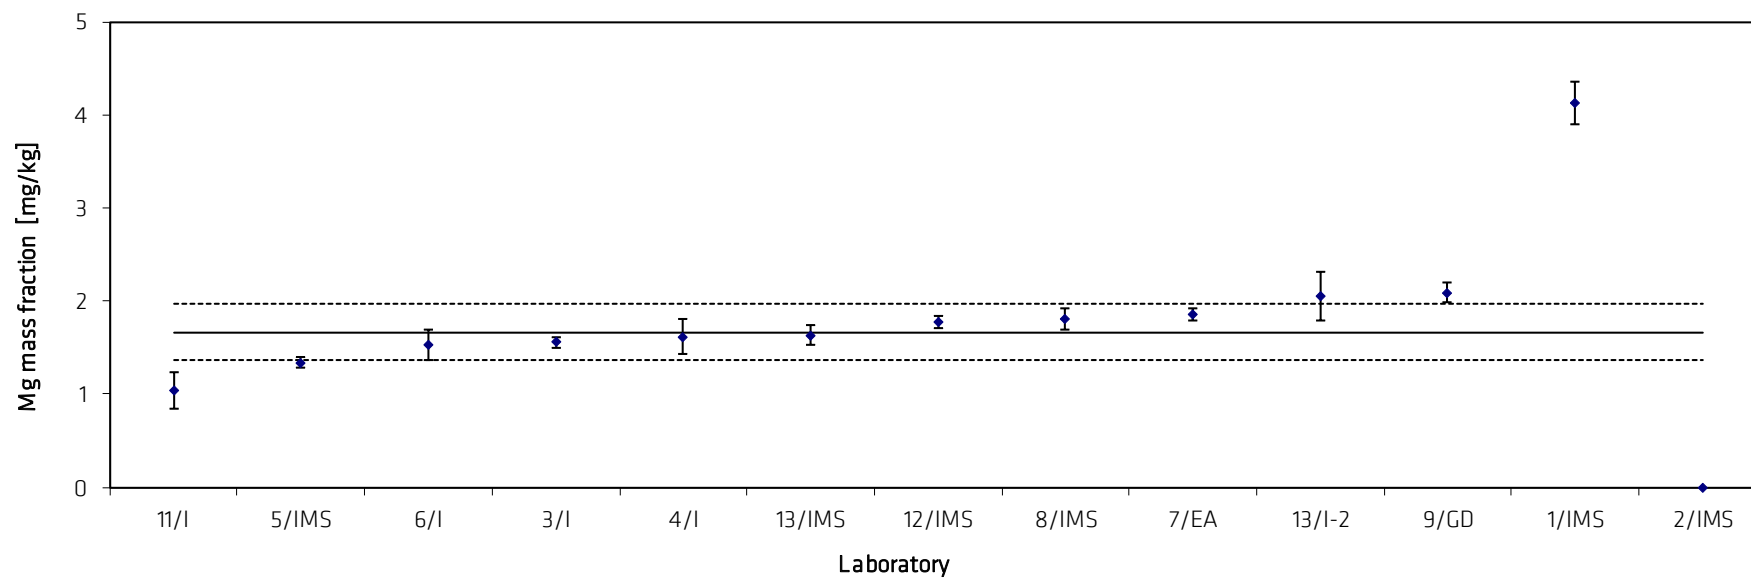


Table 11: Results for Mn in BAM-M383d

Lab./Meth.	11/I	1/IMS	4/I	13/IMS	6/I	13/I-2	8/IMS	2/IMS	5/IMS	10/I	12/IMS	9/GD	7/EA	3/I		
$M_i$ [mg/kg]	0.33	0.82	0.8	0.86	0.91	1.00	0.96	0.97	0.95	1.03	1.12	1.11	1.17	<1		$n$ 12
	0.40	0.81	0.9	0.86	0.89	1.10	0.87	0.87	1.02	1.02	1.10	1.10	1.29	<1		
	0.40	0.75	0.9	0.82	0.98	0.90	1.08	0.88	0.98	0.96	1.09	1.10	1.21	<1		
	0.41	0.80	0.8	0.89	0.82	0.90	0.89	1.05	0.88	0.92	1.11	1.10	1.27	<1		
	0.46	0.75	0.8	0.84	0.85	0.90	0.90	0.95	0.96	0.99	1.11	1.21	1.15	<1		
	0.45	0.80	0.8	0.85	0.90	0.80		0.95	0.98	0.97	1.10	1.20	1.24	<1		
												1.19				
												1.19				
$M$ [mg/kg]	<b>0.41</b>	<b>0.79</b>	<b>0.83</b>	<b>0.85</b>	<b>0.89</b>	<b>0.93</b>	<b>0.94</b>	<b>0.95</b>	<b>0.96</b>	<b>0.98</b>	<b>1.10</b>	<b>1.15</b>	<b>1.22</b>	<b>&lt;1</b>		<b>0.97</b>
$s$ [mg/kg]	0.05	0.03	0.05	0.02	0.05	0.10	0.09	0.07	0.05	0.04	0.01	0.05	0.06		$s_M$ [mg/kg]	0.131
$s_{rel}$	0.1132	0.0388	0.0620	0.0274	0.0616	0.1107	0.0906	0.0695	0.0481	0.0415	0.0106	0.0447	0.0453		$\bar{s}_i$ [mg/kg]	0.055
																0.1354

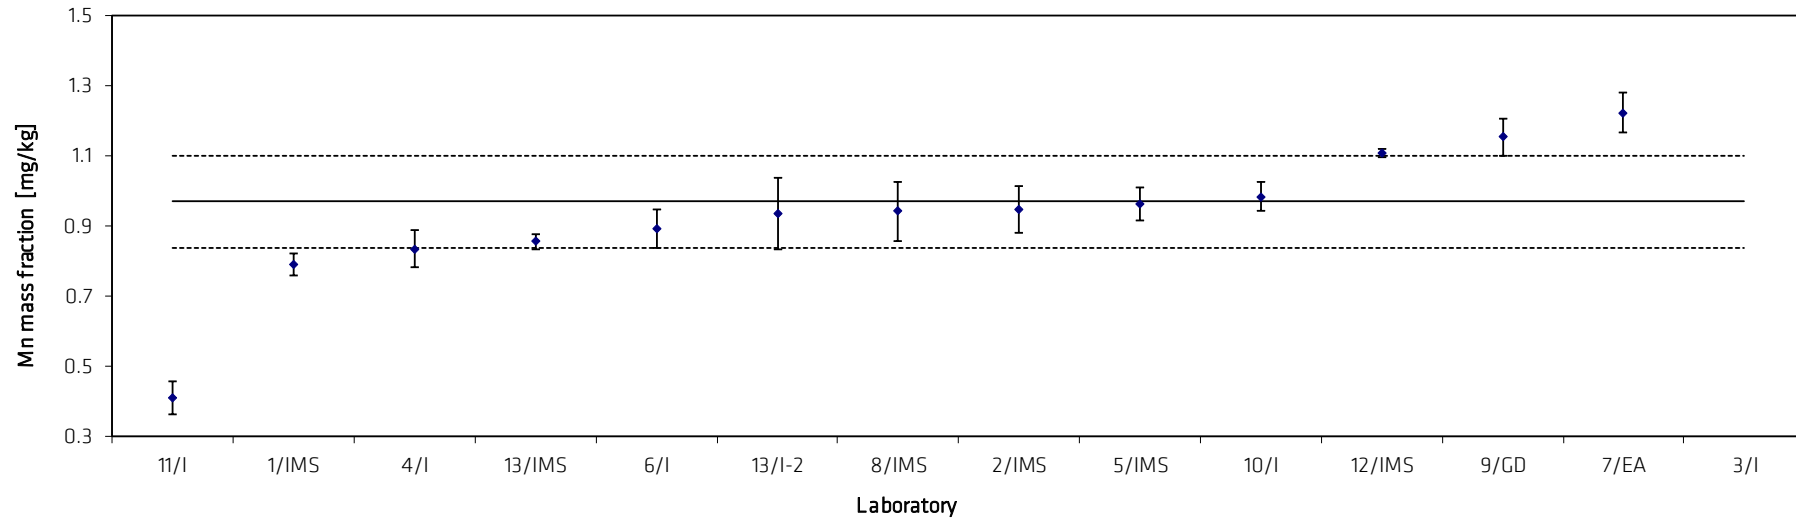


Table 12: Results for Ni in BAM-M383d

Lab./Meth.	7/EA	13/I-1	5/IMS	13/I-2	10/I	11/I	3/I	12/IMS	13/IMS	9/GD	2/IMS	1/IMS	6/I	8/IMS	4/I		
$M_i$ [mg/kg]	2.88	3.85	4.02	4.50	4.34	4.38	4.82	4.66	4.90	4.74	5.03	5.03	5.00	5.24	<2		$n$
	2.81	3.99	3.94	4.20	4.39	5.03	4.76	4.67	4.90	4.66	5.19	5.11	5.52	4.67	<2		13
	2.76	4.20	4.02	4.00	4.43	4.39	4.80	5.08	4.70	4.91	5.05	5.16	4.88	6.03	<2		
	2.90	3.75	4.06	4.10	4.52	4.50	4.77	4.74	5.00	4.70	5.43	5.07	5.01	4.95	<2		
	2.74	3.94	4.08	4.50	4.38	4.40	4.71	4.77	4.80	5.28	4.88	5.25	5.15		<2		
	2.87	3.95	4.12	4.00	4.38	4.51	4.77	5.05	4.80	5.24	5.11	5.15	5.58		<2		
										5.45							
										5.28							
$M$ [mg/kg]	<b>2.83</b>	<b>3.95</b>	<b>4.04</b>	<b>4.22</b>	<b>4.41</b>	<b>4.54</b>	<b>4.77</b>	<b>4.83</b>	<b>4.85</b>	<b>5.03</b>	<b>5.12</b>	<b>5.13</b>	<b>5.19</b>	<b>5.22</b>	<b>&lt;2</b>		<b>4.71</b>
$s$ [mg/kg]	0.07	0.15	0.06	0.23	0.06	0.25	0.04	0.19	0.10	0.32	0.18	0.08	0.29	0.59		$s_M$ [mg/kg]	0.44
$s_{rel}$	0.0236	0.0383	0.0158	0.0549	0.0142	0.0549	0.0079	0.0387	0.0216	0.0626	0.0361	0.0150	0.0563	0.1123		$\bar{s}_i$ [mg/kg]	0.23
																	0.0943

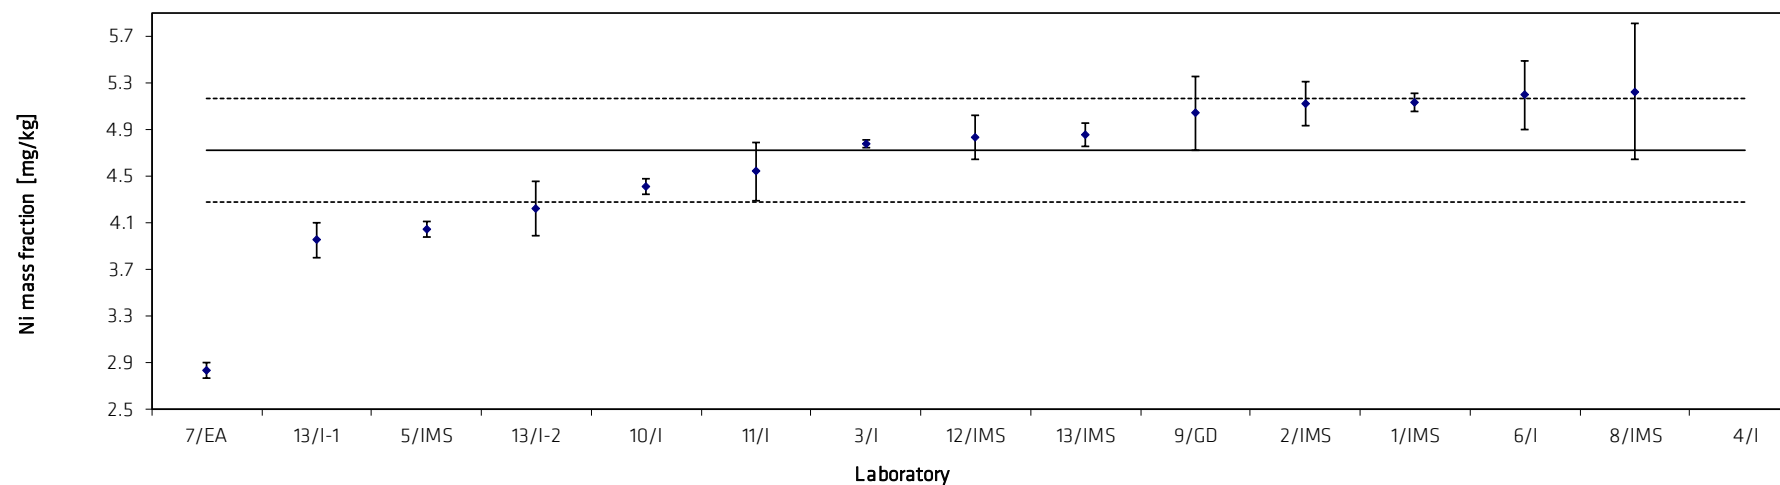


Table 13: Results for P in BAM-M383d

Lab./Meth.	11/l	10/l	9/GD	3/l	5/l	13/l-2	4/l	2/l		
$M_i$ [mg/kg]	0.51	0.54	0.97	<1	<1	<2	<5	<5		$n$ 3
	0.35	0.24	0.84	<1	<1	<2	<5	<5		
	0.16	0.79	0.85	<1	<1	<2	<5	<5		
		0.34	0.84	<1	<1	<2	<5	<5		
		0.45	0.54	<1	<1	<2	<5	<5		
		0.41	0.51	<1	<1	<2	<5	<5		
			0.53							
		0.49								
$M$ [mg/kg]	<b>0.34</b>	<b>0.46</b>	<b>0.76</b>	<1	<1	<2	<5	<5		<b>0.5</b>
$s$ [mg/kg]	0.18	0.19	0.18						$s_M$ [mg/kg]	0.22
$s_{rel}$	0.5153	0.4118	0.2440						$\bar{s}_i$ [mg/kg]	0.11
										0.4136

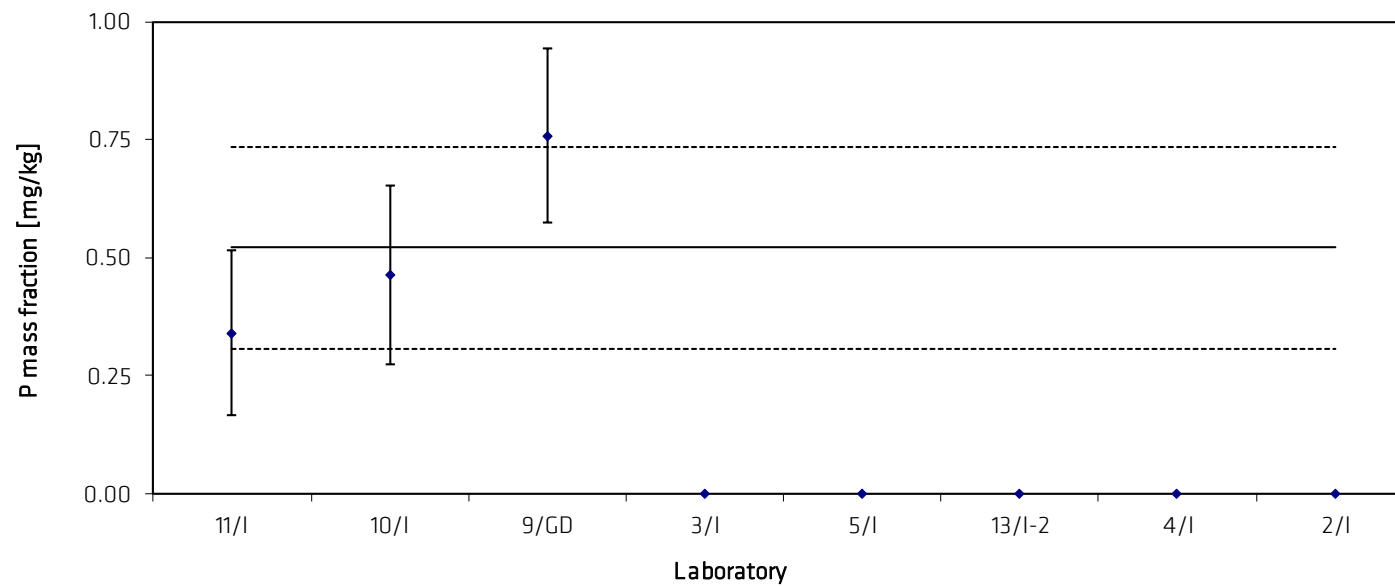


Table 14: Results for Pb in BAM-M383d

Lab./Meth.	6/I	4/I	7/EA	11/I	9/GD	1/IMS	12/IMS	9/EA	5/IMS	8/IMS	13/I-1	13/I-2	13/IMS	2/IMS	3/I		
$M_i$ [mg/kg]	1.29	5.3	5.8	6.3	7.17	7.51	7.40	7.50	7.75	8.78	8.40	8.90	9.20	10.29	12.90		$n$ 13
	1.23	5.4	5.7	6.1	7.53	7.57	7.77	8.13	7.57	7.25	8.38	8.50	8.70	10.24	13.54		
	1.29	5.4	5.7	6.1	7.15	7.62	8.07	8.14	7.93	8.80	8.48	8.90	9.00	10.34	12.90		
	1.14	4.8	5.9	6.3	7.66	7.75	8.01	7.87	8.08	8.38	8.77	8.30	8.60	10.56	13.18		
	1.00	4.8	5.8	5.9	7.07	7.86	7.79	7.70	7.88		8.64	8.90	9.10	11.80	12.30		
	1.10	4.9	5.8	6.1	7.35	7.76	7.60	7.82	7.98		8.49	9.60	9.30	10.49	13.09		
					7.43												
					7.49												
$M$ [mg/kg]	1.18	5.10	5.76	6.14	7.32	7.68	7.77	7.86	7.86	8.30	8.53	8.85	8.98	10.62	12.99		7.75
$s$ [mg/kg]	0.12	0.30	0.07	0.16	0.23	0.13	0.25	0.25	0.18	0.73	0.15	0.45	0.28	0.59	0.4	$s_M$ [mg/kg]	1.46
$s_{rel}$	0.0985	0.0582	0.0125	0.0254	0.0319	0.0173	0.0325	0.0315	0.0230	0.0877	0.0176	0.0504	0.0310	0.0558	0.0316	$\bar{s}_i$ [mg/kg]	0.34
																	0.1887

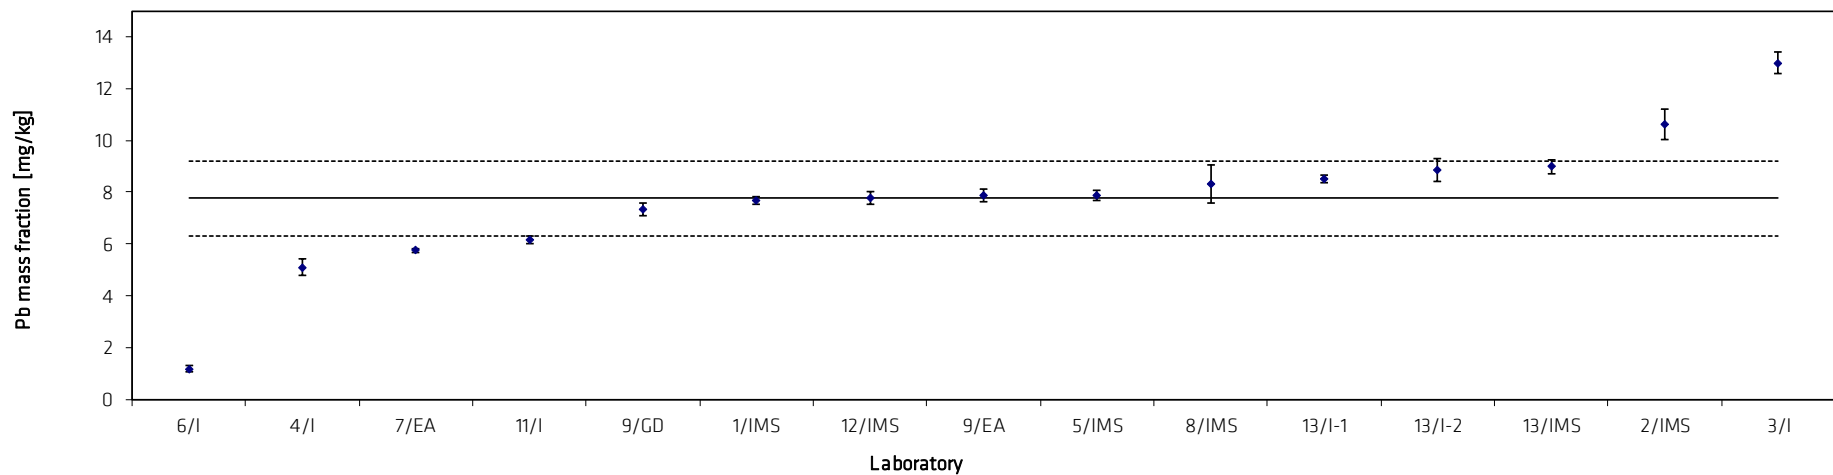


Table 15: Results for S in BAM-M383d

Lab./Meth.	6/I	13/I-2	3/I	9/GD	9/V	7/V	4/I		
$M_i$ [mg/kg]	3.08	3.17	3.37	[5.59]	3.50	4.00	<10		$n$
	1.21	3.28	3.08	4.03	4.10	4.40	<10		6
	3.22	2.97	3.19	3.58	4.00	4.40	<10		
	2.08	3.10	3.05	3.43	3.90	4.40	<10		
	3.83	3.20	3.06	3.82	3.70	4.00	<10		
	2.01	3.06	3.11	3.65	4.40	4.40	<10		
				3.78					
				3.57					
$M$ [mg/kg]	<b>2.57</b>	<b>3.13</b>	<b>3.14</b>	<b>3.69</b>	<b>4.02</b>	<b>4.32</b>	<b>&lt;10</b>		<b>3.48</b>
$s$ [mg/kg]	0.97	0.11	0.12	0.20	0.26	0.18		$s_M$ [mg/kg]	0.649
$s_{rel}$	0.3759	0.0351	0.0388	0.0539	0.0644	0.0414		$\bar{s}_i$ [mg/kg]	0.396
									0.1864

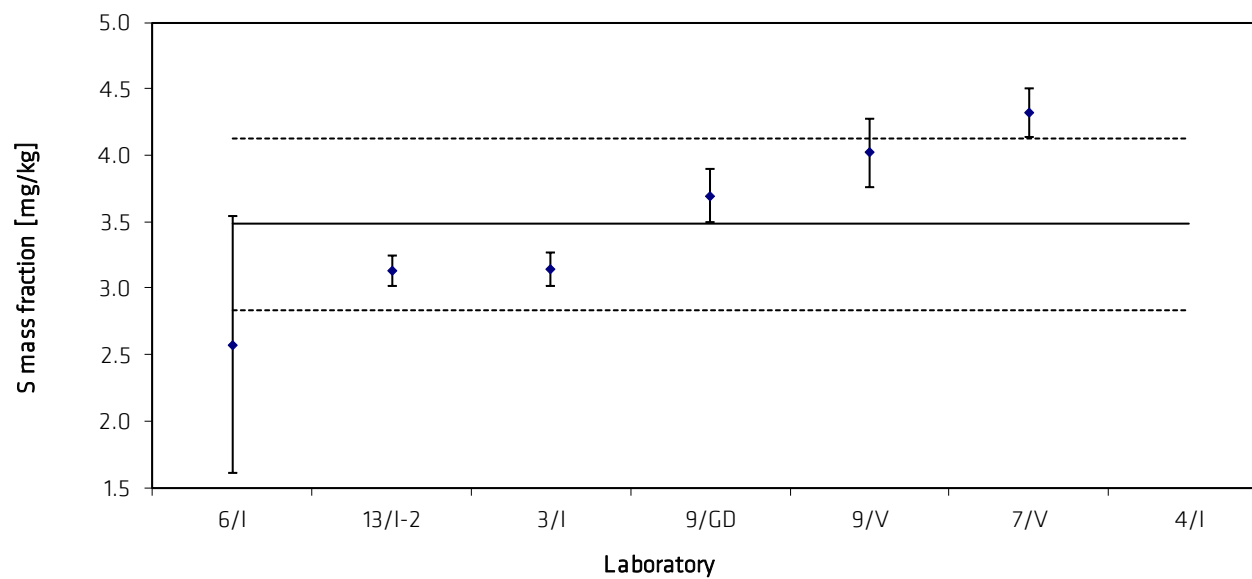


Table 16: Results for Sb in BAM-M383d

Lab./Meth.	2/IMS	1/IMS	3/I	4/I	9/GD	12/IMS	5/IMS	13/IMS	8/IMS	7/EA	13/I-2	6/I		
$M_i$ [mg/kg]	1.40	1.68	1.56	1.8	1.72	1.73	1.58	1.76	1.92	2.04	2.30	2.86		$n$
	1.35	1.63	1.78	1.5	1.76	1.74	1.95	1.78	1.89	2.15	2.50	2.95		11
	1.35	1.66	1.75	1.8	1.69	1.67	1.59	1.75	1.94	2.22	2.20	2.65		
	1.54	1.68	1.75	1.7	1.75	1.76	1.84	1.75	1.94	2.11	2.00	3.12		
	1.34	1.69	1.67	1.7	1.69	1.74	1.83	1.78	1.86	2.07	1.90	3.18		
	1.30	1.64	1.55	1.6	1.74	1.74	1.82	1.80	1.95	2.20	1.90	3.09		
					1.71	1.73								
$M$ [mg/kg]	1.38	1.66	1.68	1.68	1.72	1.73	1.77	1.77	1.92	2.13	2.13	2.98		1.78
$s$ [mg/kg]	0.08	0.02	0.10	0.12	0.03	0.03	0.15	0.02	0.04	0.07	0.24	0.20	$s_M$ [mg/kg]	0.216
$s_{rel}$	0.0595	0.0146	0.0603	0.0694	0.0147	0.0182	0.0851	0.0113	0.0183	0.0335	0.1135	0.0665	$\bar{s}_i$ [mg/kg]	0.105
														0.1215

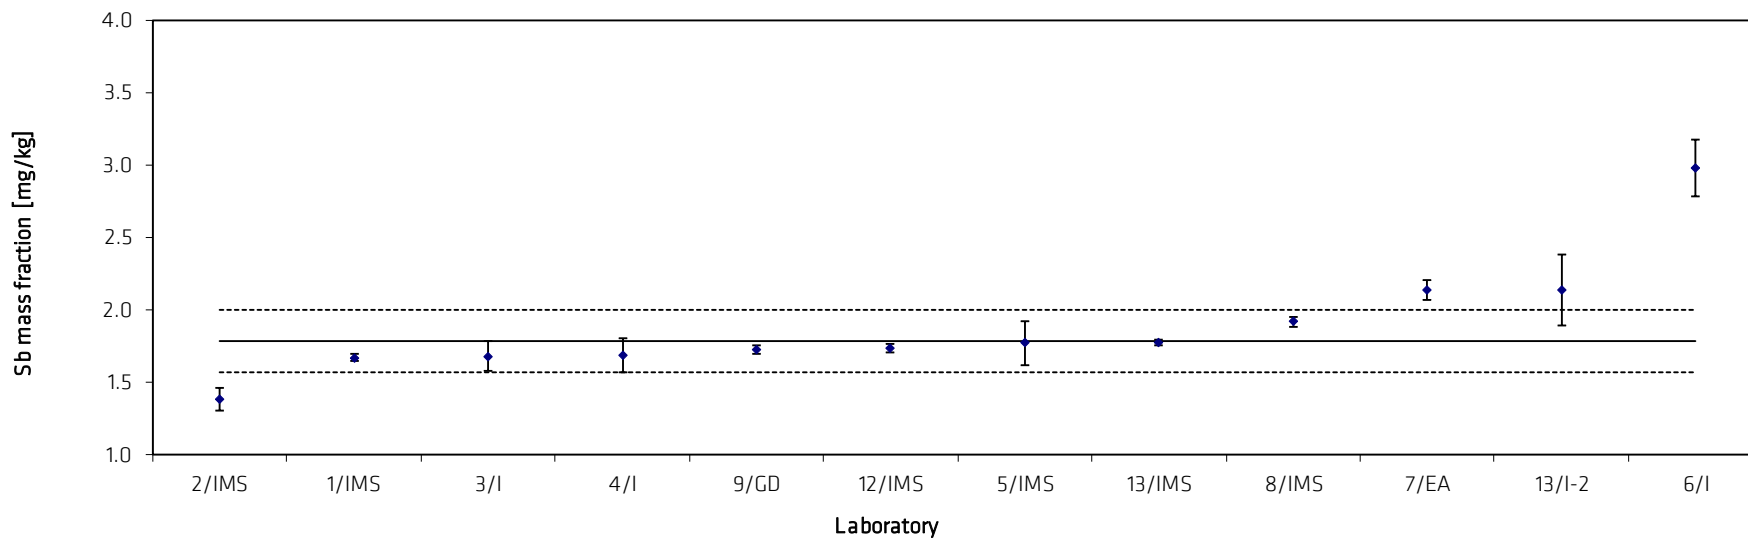




Table 17: Results for Se in BAM-M383d

Lab./Meth.	1/IMS	9/GD	12/IMS	8/IMS	11/I	7/EA	5/IMS	2/IMS	3/I	4/I		
$M_i$ [mg/kg]	0.20	0.24	0.28	0.63	1.02	1.24	<0.3	<0.5	<1	<1		$n$
	0.20	0.26	0.33	0.57	0.76	1.12	<0.3	<0.5	<1	<1		6
	0.26	0.26	0.37	0.54	0.84	1.15	<0.3	<0.5	<1	<1		
	0.31	0.25	0.39	0.59	0.77	1.21	<0.3	<0.5	<1	<1		
	0.26	0.25	0.29	0.61	0.72	1.11	<0.3	<0.5	<1	<1		
	0.15	0.27	0.34	0.58	0.79	1.23	<0.3	<0.5	<1	<1		
		0.27										
		0.27										
$M$ [mg/kg]	<b>0.23</b>	<b>0.26</b>	<b>0.33</b>	<b>0.59</b>	<b>0.82</b>	<b>1.18</b>	<b>&lt;0.3</b>	<b>&lt;0.5</b>	<b>&lt;1</b>	<b>&lt;1</b>		<b>0.57</b>
$s$ [mg/kg]	0.06	0.01	0.04	0.03	0.11	0.06					$s_M$ [mg/kg]	0.374
$s_{rel}$	0.2490	0.0442	0.1279	0.0535	0.1311	0.0486					$\bar{s}_i$ [mg/kg]	0.046
												0.6596

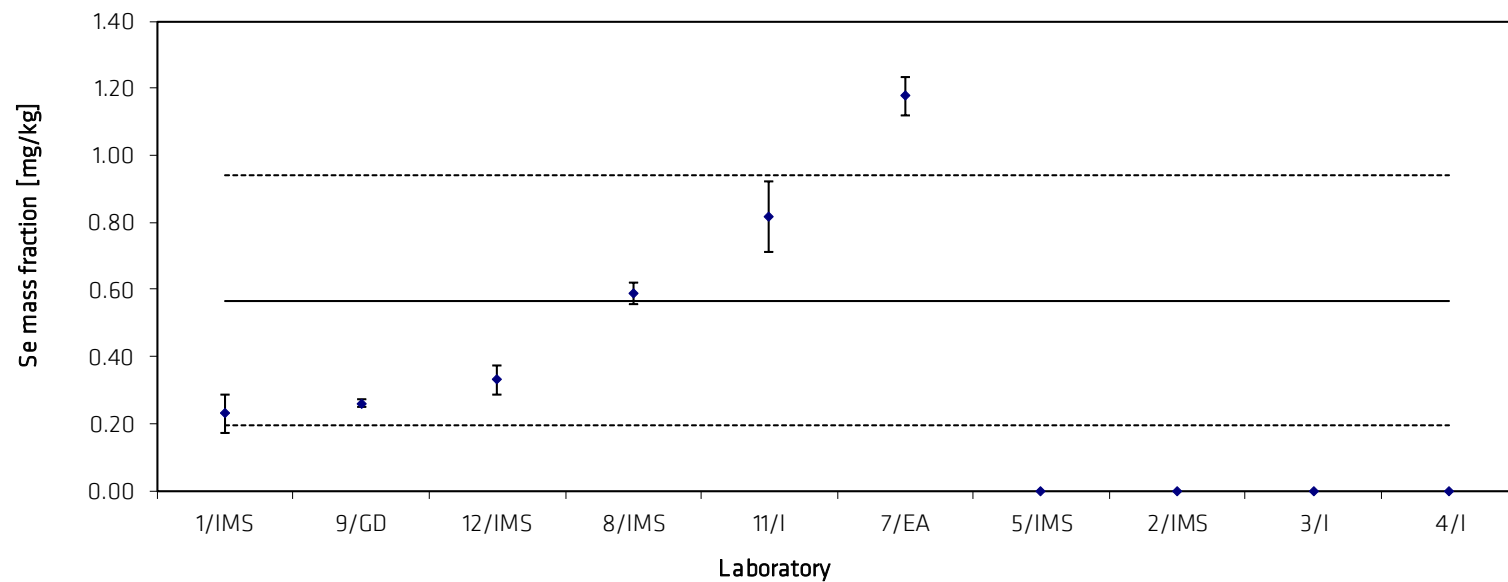


Table 18: Results for Sn in BAM-M383d

Lab./Meth.	6/I	4/I	2/IMS	1/IMS	12/IMS	5/IMS	13/I-2	9/EA	3/I	13/IMS	13/I-1	9/GD	7/EA	8/IMS	10/I		
$M_i$ [mg/kg]	3.12	3.3	2.70	3.42	4.01	3.65	3.70	4.00	4.02	4.15	3.98	4.19	4.12	4.14	4.34		$n$
	2.90	3.0	2.97	3.27	3.81	3.85	4.00	4.43	3.97	4.20	4.02	4.33	4.28	4.43	4.53		15
	2.86	3.3	2.97	3.52	3.06	3.73	4.10	4.20	3.99	4.15	4.27	4.17	4.31	4.43	4.60		
	3.10	2.9	3.19	3.31	3.44	3.49	3.70	3.66	3.98	4.25	4.00	4.34	4.20	4.47	4.26		
	3.04	3.0	3.77	3.45	3.68	3.71	3.80	3.71	3.98	4.17	4.31	4.07	4.16	4.47	4.30		
	3.07	2.9	2.91	3.50	3.95	3.68	3.90	3.25	4.00	4.15	4.51	4.19	4.23		4.36		
												4.11					
												4.20					
$M$ [mg/kg]	<b>3.02</b>	<b>3.07</b>	<b>3.09</b>	<b>3.41</b>	<b>3.66</b>	<b>3.68</b>	<b>3.87</b>	<b>3.88</b>	<b>3.99</b>	<b>4.18</b>	<b>4.18</b>	<b>4.20</b>	<b>4.22</b>	<b>4.39</b>	<b>4.40</b>		<b>3.81</b>
$s$ [mg/kg]	0.11	0.19	0.37	0.10	0.36	0.12	0.16	0.42	0.02	0.04	0.22	0.09	0.07	0.14	0.14	$s_M$ [mg/kg]	0.48
$s_{rel}$	0.0361	0.0607	0.1199	0.0297	0.0977	0.0321	0.0422	0.1091	0.0045	0.0096	0.0515	0.0226	0.0170	0.0319	0.0308	$\bar{s}_i$ [mg/kg]	0.21
																	0.1257

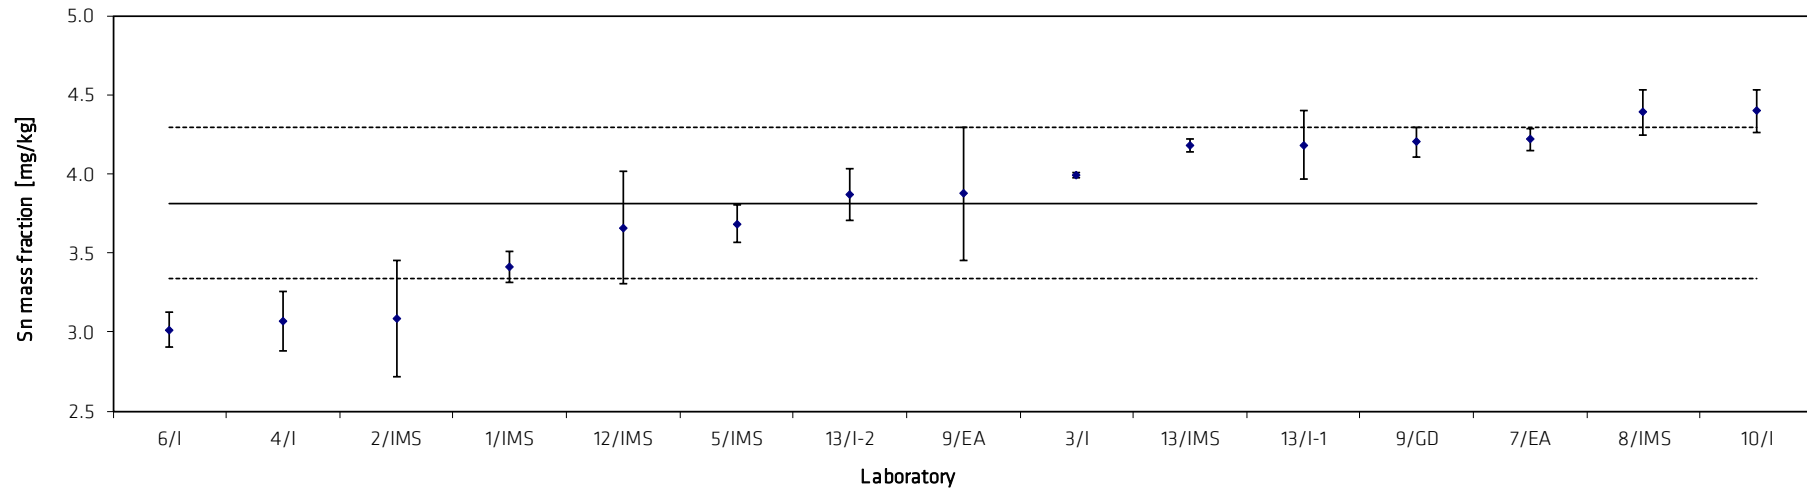


Table 19: Results for Te in BAM-M383d

Lab./Meth.	9/GD	1/IMS	2/IMS	8/IMS	12/IMS	13/IMS	5/IMS	7/EA	3/I	4/I		
$M_i$ [mg/kg]	0.42	0.46	0.49	0.49	0.49	0.54	0.95	1.21	<1	<2		$n$
	0.43	0.48	0.54	0.51	0.50	0.50	0.95	1.12	<1	<2		6
	0.42	0.42	0.43	0.52	0.48	0.51	0.97	1.15	<1	<2		
	0.43	0.45	0.47	0.50	0.50	0.44	0.90	1.26	<1	<2		
	0.44	0.40	0.44	0.47	0.51	0.49	0.92	1.20	1.03	<2		
	0.44	0.45	0.50	0.41	0.50	0.55	0.95	1.27	<1	<2		
	0.44											
	0.44											
$M$ [mg/kg]	<b>0.43</b>	<b>0.44</b>	<b>0.48</b>	<b>0.48</b>	<b>0.50</b>	<b>0.51</b>	<b>0.94</b>	<b>1.20</b>	<1	<2		<b>0.47</b>
$s$ [mg/kg]	0.01	0.03	0.04	0.04	0.01	0.04	0.03	0.06			$s_M$ [mg/kg]	0.029
$s_{rel}$	0.024	0.065	0.083	0.082	0.019	0.078	0.029	0.049			$\bar{s}_i$ [mg/kg]	0.031
												0.062

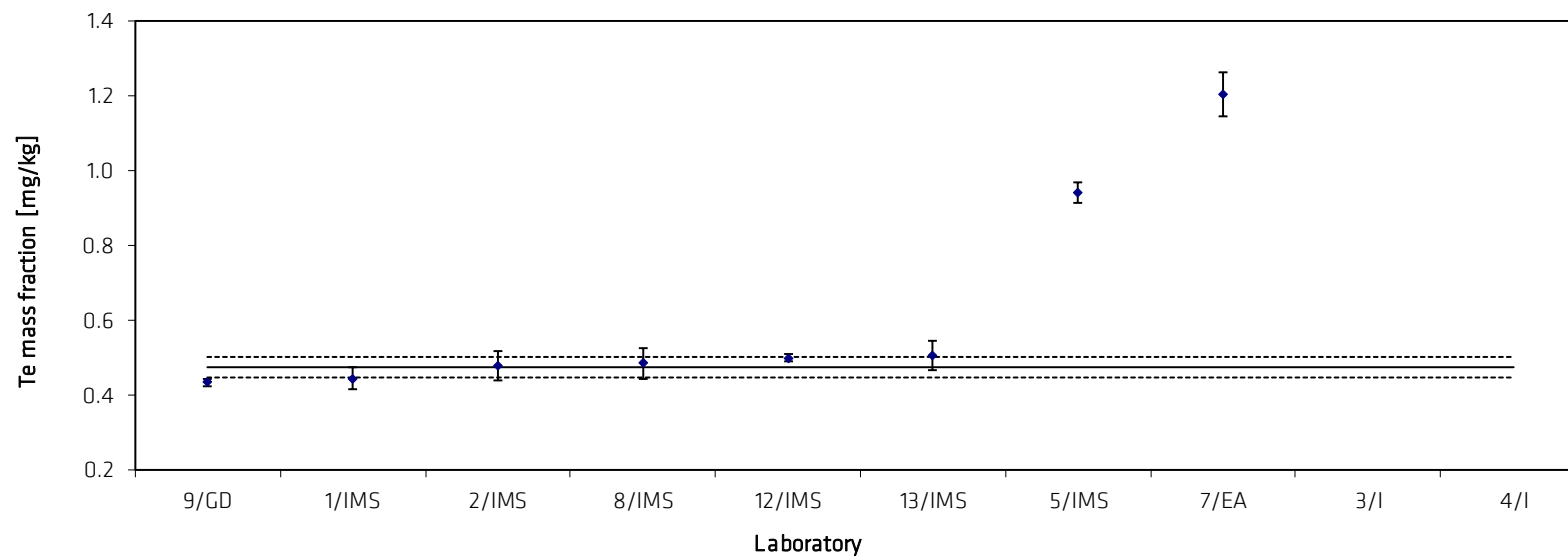


Table 20: Results for Ti in BAM-M383d

Lab./Meth.	11/I	1/IMS	13/I-2	13/IMS	6/I	9/GD	10/I	12/IMS	4/I	8/IMS	3/I		
$M_i$ [mg/kg]	0.41	0.80	1.10	1.10	1.20	1.19	1.32	1.43	1.3	1.6	1.03		$n$ 10
	0.63	0.73	1.10	1.20	1.20	1.22	1.30	1.41	1.6	1.7	<1		
	0.46	0.78	1.10	1.10	1.33	1.19	1.41	1.44	1.6	1.6	<1		
	0.54	0.70	1.00	1.30	1.17	1.24	1.39	1.42	1.3	1.7	<1		
	0.67	0.75	0.90	1.20	1.12	1.29	1.45	1.41	1.4	1.6	<1		
	0.62	0.75	0.90	1.20	1.18	1.32	1.47	1.42	1.4		<1		
						1.26							
						1.33							
$M$ [mg/kg]	<b>0.56</b>	<b>0.75</b>	<b>1.02</b>	<b>1.18</b>	<b>1.20</b>	<b>1.25</b>	<b>1.39</b>	<b>1.42</b>	<b>1.43</b>	<b>1.63</b>	<b>&lt;1</b>		<b>1.18</b>
$s$ [mg/kg]	0.10	0.04	0.10	0.08	0.07	0.06	0.07	0.01	0.14	0.03		$s_M$ [mg/kg]	0.329
$s_{rel}$	0.186	0.047	0.097	0.064	0.058	0.045	0.049	0.007	0.095	0.018		$\bar{s}_i$ [mg/kg]	0.074
													0.278

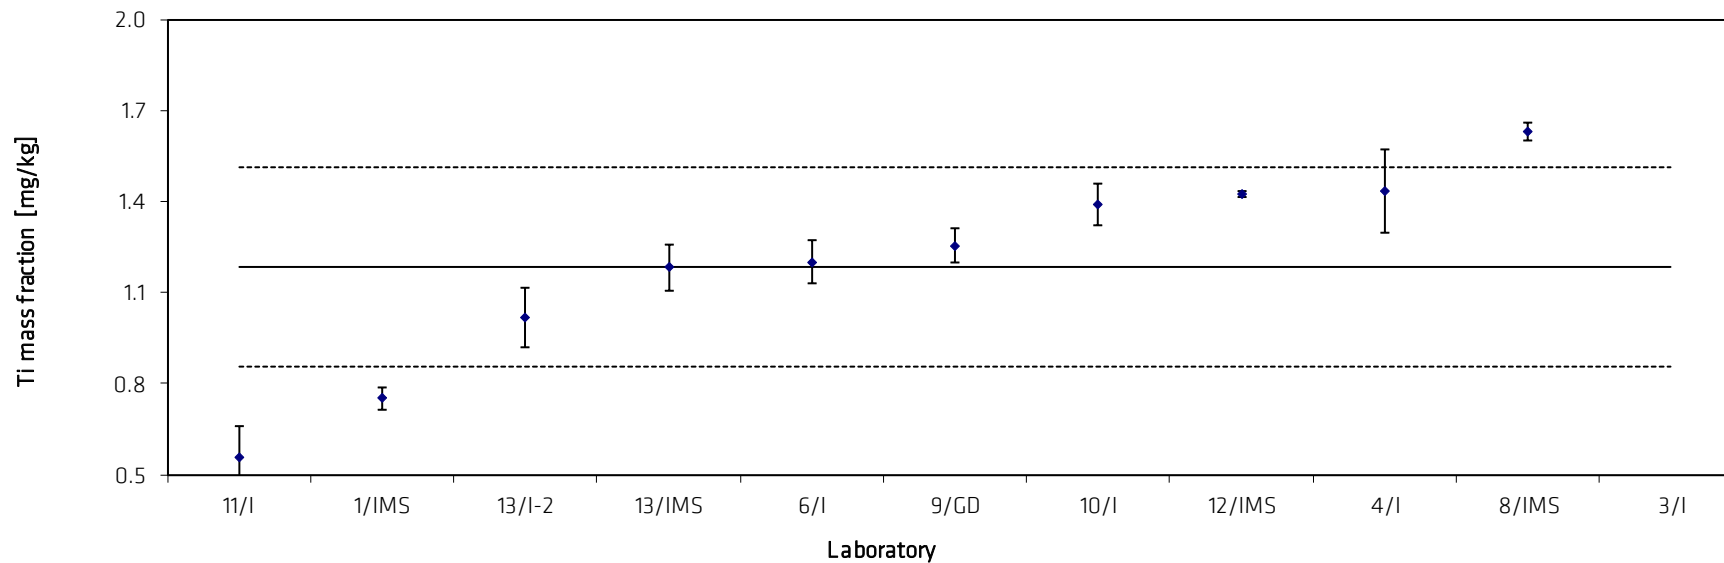


Table 21: Results for Zn in BAM-M383d

Lab./Meth.	5/IMS	13/I-1	12/IMS	13/IMS	8/IMS	9/GD	1/IMS	6/I	7/EA	4/I	3/I	2/IMS			
$M_i$ [mg/kg]	0.93	0.91	1.01	0.87	1.01	1.19	1.28	1.53	1.92	<0.5	<1	<5		$n$	
	0.92	0.90	0.96	0.99	1.08	1.17	1.16	1.11	1.80	<0.5	<1	<5		8	
	0.95	0.87	0.97	0.89	1.08	1.19	1.22	1.45	1.95	<0.5	<1	<5			
	0.90	0.89	0.96	1.14		1.12	1.19	1.57	1.83	<0.5	<1	<5			
	0.95	1.10	1.05	1.03		1.26	1.23	1.29	1.79	<0.5	<1	<5			
	0.88	0.90	0.97	1.00		1.18	1.09	1.31	1.90	<0.5	<1	<5			
							1.21								
							1.08								
$M$ [mg/kg]	<b>0.92</b>	<b>0.93</b>	<b>0.99</b>	<b>0.99</b>	<b>1.06</b>	<b>1.17</b>	<b>1.20</b>	<b>1.38</b>	<b>1.87</b>	<b>&lt;0.5</b>	<b>&lt;1</b>	<b>&lt;5</b>		<b>1.08</b>	
$s$ [mg/kg]	0.03	0.09	0.04	0.10	0.04	0.05	0.07	0.17	0.07				$s_M$ [mg/kg]	0.159	
$s_{rel}$	0.0310	0.0918	0.0357	0.0999	0.0382	0.0461	0.0547	0.1255	0.0360				$\bar{s}_i$ [mg/kg]	0.085	
														0.1471	


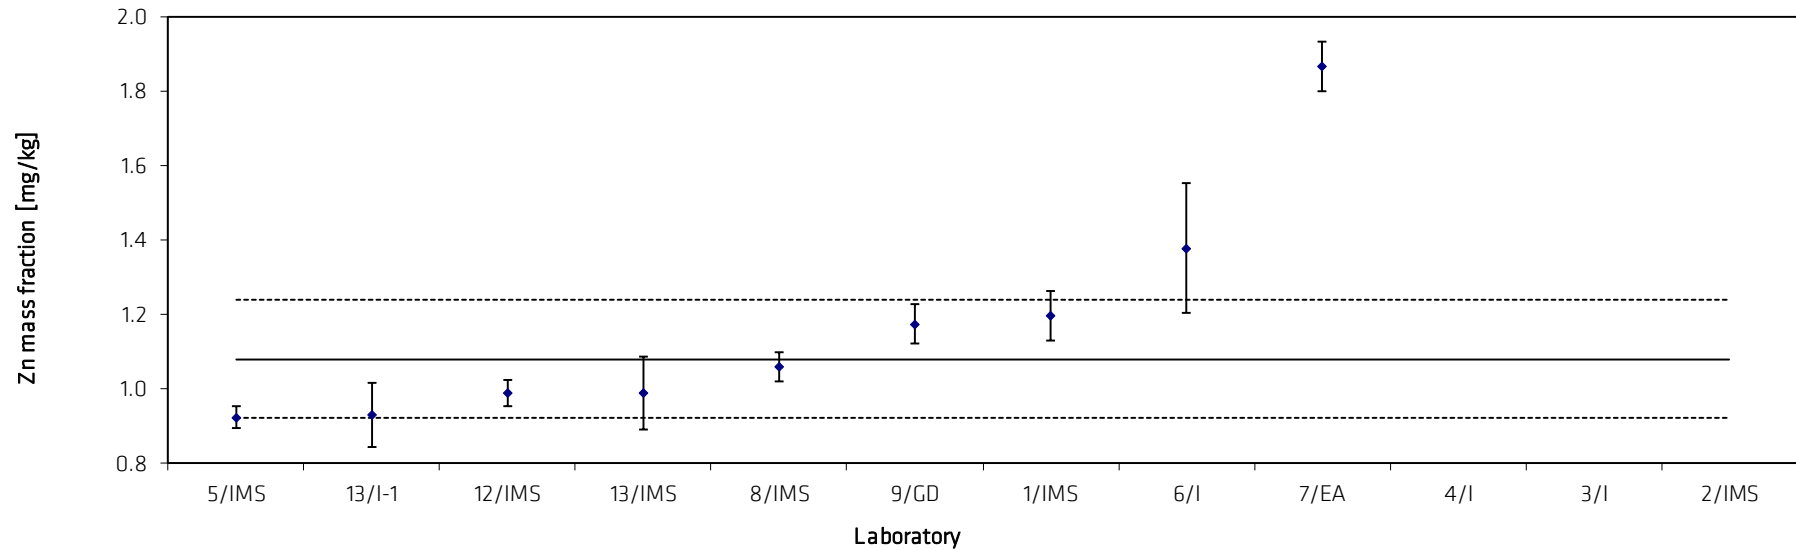


Table 22: Results for Zr in BAM-M383d

Lab./Meth.	6/I	11/I	8/IMS	9/GD	1/IMS	12/IMS	13/IMS	4/I	3/I	2/I		
$M_i$ [mg/kg]	0.07	0.35	1.11	0.004	<0.1	<0.1	<0.1	<0.5	<1	<1		$n$
	0.01	0.72	1.02	0.012	<0.1	<0.1	<0.1	<0.5	<1	<1		3
	0.02	0.38	1.04	0.005	<0.1	<0.1	<0.1	<0.5	<1	<1		
	0.07	0.45	1.12	0.004	<0.1	<0.1	<0.1	<0.5	<1	<1		
	0.04	0.35		0.014	<0.1	<0.1	<0.1	<0.5	<1	<1		
	0.04	0.27		0.016	<0.1	<0.1	<0.1	<0.5	<1	<1		
			0.009									
			0.011									
$M$ [mg/kg]	0.04	0.42	1.07	< 0.05	<0.1	<0.1	<0.1	<0.5	<1	<1		0.51
$s$ [mg/kg]	0.0	0.2	0.0								$s_M$ [mg/kg]	0.52
$s_{rel}$	0.5960	0.3762	0.0465								$\bar{s}_i$ [mg/kg]	0.05
												1.0197

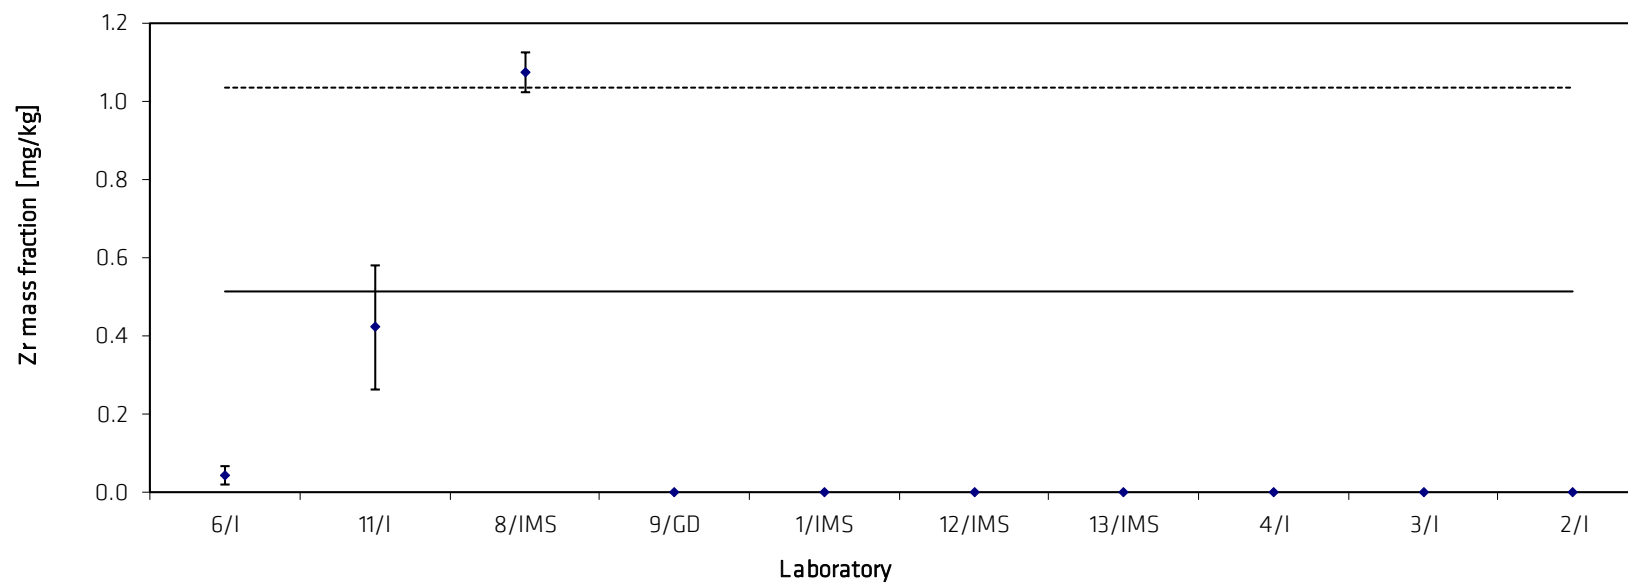

The data was statistically evaluated to detect outlying values (Grubbs, Nalimov, Dixon, Cochran). The Cochran-test was performed only once. The following results were obtained:

Tab. 23: Outcome of statistical tests on the results obtained for Ag

	1 <sup>st</sup> run	2 <sup>nd</sup> run
Number of data sets	14	13
Scheffe's test (data compatible?)	yes	yes
Snedecor-F-Test and Bartlett-Test	Pooling not allowed	Pooling not allowed
Dixon ( $\alpha = 0.05$ )	Lab. 11	---
Dixon ( $\alpha = 0.01$ )	---	---
Nalimov ( $\alpha = 0.05$ )	Lab. 11	Lab. 6
Nalimov ( $\alpha = 0.01$ )	Lab. 11	---
Grubbs ( $\alpha = 0.05$ )	Lab. 11	---
Grubbs ( $\alpha = 0.01$ )	---	---
Grubbs Pair ( $\alpha = 0.05$ )	Labs. 11 and 6	---
Grubbs Pair ( $\alpha = 0.01$ )	---	---
Cochran ( $\alpha = 0.01$ )	Lab. 8	Lab. 8
Kolmogorov-Smirnov-Lilliefors Test	Distribution: normal	Distribution: normal

The outlier (Lab. 11, 1<sup>st</sup> run) was removed.

Tab. 24: Outcome of statistical tests on the results obtained for As (" $<$ -values" were not considered)

	1 <sup>st</sup> run	2 <sup>nd</sup> run
Number of data sets	14	13
Scheffe's test (data compatible?)	yes	yes
Snedecor-F-Test and Bartlett-Test	Pooling not allowed	Pooling not allowed
Dixon ( $\alpha = 0.05$ )	Labs. 9/EA	---
Dixon ( $\alpha = 0.01$ )	Lab. 9/EA	---
Nalimov ( $\alpha = 0.05$ )	Lab. 9/EA	Lab. 6
Nalimov ( $\alpha = 0.01$ )	Lab. 9/EA	---
Grubbs ( $\alpha = 0.05$ )	Lab. 9/EA	---
Grubbs ( $\alpha = 0.01$ )	Lab. 9/EA	---
Grubbs Pair ( $\alpha = 0.05$ )	---	---
Grubbs Pair ( $\alpha = 0.01$ )	---	---
Cochran	Lab. 8	Lab. 8
Kolmogorov-Smirnov-Lilliefors Test	Distribution: normal	Distribution: normal

The outlier (Lab. 9/EA, 1<sup>st</sup> run) was removed, the Cochran outlier was not removed.

Tab. 25: Outcome of statistical tests on the results obtained Cd (“<-values” were not considered)

	1 <sup>st</sup> run	2 <sup>nd</sup> run
Number of data sets	15	14
Scheffe’s test (data compatible?)	yes	yes
Snedecor-F-Test and Bartlett-Test	Pooling not allowed	Pooling not allowed
Dixon ( $\alpha = 0.05$ )	Lab. 7	---
Dixon ( $\alpha = 0.01$ )	---	---
Nalimov ( $\alpha = 0.05$ )	Lab. 7	Labs. 4 and 13/1-2
Nalimov ( $\alpha = 0.01$ )	Lab. 7	---
Grubbs ( $\alpha = 0.05$ )	Lab. 7	---
Grubbs ( $\alpha = 0.01$ )	Lab. 7	---
Grubbs Pair ( $\alpha = 0.05$ )	---	---
Grubbs Pair ( $\alpha = 0.01$ )	---	---
Cochran	Lab. 8	Lab. 8
Kolmogorov-Smirnov-Lilliefors Test	Distribution: normal	Distribution: normal

The outlier (Lab. 7, 1<sup>st</sup> run) was removed, the Cochran outlier was not removed.

Tab. 26: Outcome of statistical tests on the results obtained for Cr

	1 <sup>st</sup> run	2 <sup>nd</sup> run
Number of data sets	14	13
Scheffe’s test (data compatible?)	yes	yes
Snedecor-F-Test and Bartlett-Test	Pooling not allowed	Pooling not allowed
Dixon ( $\alpha = 0.05$ )	---	---
Dixon ( $\alpha = 0.01$ )	---	---
Nalimov ( $\alpha = 0.05$ )	Lab. 11	Labs. 1 and 7
Nalimov ( $\alpha = 0.01$ )	---	---
Grubbs ( $\alpha = 0.05$ )	---	---
Grubbs ( $\alpha = 0.01$ )	---	---
Grubbs Pair ( $\alpha = 0.05$ )	---	---
Grubbs Pair ( $\alpha = 0.01$ )	---	---
Cochran ( $\alpha = 0.01$ )	Lab. 1	Lab. 1
Kolmogorov-Smirnov-Lilliefors Test	Distribution: normal	Distribution: normal

The outlier (Lab. 11, 1<sup>st</sup> run and Lab. 1) were removed, because there seem to be insoluble parts not considered.



Tab. 27: Outcome of statistical tests on the results obtained for Bi and Se (“<-values” were not considered)

	Bi	Se
Number of data sets	7	7
Scheffe's test (data compatible?)	yes	yes
Snedecor-F-Test and Bartlett-Test	Pooling not allowed	Pooling not allowed
Dixon ( $\alpha = 0.05$ )	---	---
Dixon ( $\alpha = 0.01$ )	---	---
Nalimov ( $\alpha = 0.05$ )	---	---
Nalimov ( $\alpha = 0.01$ )	---	---
Grubbs ( $\alpha = 0.05$ )	---	---
Grubbs ( $\alpha = 0.01$ )	---	---
Grubbs Pair ( $\alpha = 0.05$ )	---	---
Grubbs Pair ( $\alpha = 0.01$ )	---	---
Cochran	---	Lab. 11
Kolmogorov-Smirnov-Lilliefors Test	Distribution: normal	Distribution: normal

The outlier (Se) was not removed.

Tab. 28: Outcome of statistical tests on the results obtained for Co (“<-values” were not considered)

	1 <sup>st</sup> run	2 <sup>nd</sup> run
Number of data sets	15	14
Scheffe's test (data compatible?)	yes	yes
Snedecor-F-Test and Bartlett-Test	Pooling not allowed	Pooling not allowed
Dixon ( $\alpha = 0.05$ )	Lab. 7	---
Dixon ( $\alpha = 0.01$ )	Lab. 7	---
Nalimov ( $\alpha = 0.05$ )	Lab. 7	Lab. 10
Nalimov ( $\alpha = 0.01$ )	Lab. 7	---
Grubbs ( $\alpha = 0.05$ )	Lab. 7	---
Grubbs ( $\alpha = 0.01$ )	Lab. 7	---
Grubbs Pair ( $\alpha = 0.05$ )	---	---
Grubbs Pair ( $\alpha = 0.01$ )	---	---
Cochran	Lab. 13/I-2	Lab. 13/I-2
Kolmogorov-Smirnov-Lilliefors Test	Distribution: normal	Distribution: normal

The outlier (Lab. 7, 1<sup>st</sup> run) was removed, the outliers (Lab. 10, 2<sup>nd</sup> run, Lab. 13) were not removed.

Tab. 29: Outcome of statistical tests on the results obtained for Fe

	1 <sup>st</sup> run	2 <sup>nd</sup> run
Number of data sets	14	13
Scheffe's test (data compatible?)	yes	yes
Snedecor-F-Test and Bartlett-Test	Pooling not allowed	Pooling not allowed
Dixon ( $\alpha = 0.05$ )	---	---
Dixon ( $\alpha = 0.01$ )	---	---
Nalimov ( $\alpha = 0.05$ )	Lab. 11	---
Nalimov ( $\alpha = 0.01$ )	Lab. 11	---
Grubbs ( $\alpha = 0.05$ )	---	---
Grubbs ( $\alpha = 0.01$ )	---	---
Grubbs Pair ( $\alpha = 0.05$ )	---	---
Grubbs Pair ( $\alpha = 0.01$ )	---	---
Cochran	Lab. 2	Lab. 2
Kolmogorov-Smirnov-Lilliefors Test	Distribution: normal	Distribution: normal

The outlier (Lab. 11, 1<sup>st</sup> run) was removed, the Cochran outlier was not removed.

Tab. 30: Outcome of statistical tests on the results obtained for Mg

	1 <sup>st</sup> run	2 <sup>nd</sup> run
Number of data sets	12	11
Scheffe's test (data compatible?)	yes	yes
Snedecor-F-Test and Bartlett-Test	Pooling not allowed	Pooling not allowed
Dixon ( $\alpha = 0.05$ )	Lab. 1	---
Dixon ( $\alpha = 0.01$ )	Lab. 1	---
Nalimov ( $\alpha = 0.05$ )	Lab. 1	Lab. 11
Nalimov ( $\alpha = 0.01$ )	Lab. 1	---
Grubbs ( $\alpha = 0.05$ )	Lab. 1	---
Grubbs ( $\alpha = 0.01$ )	Lab. 1	---
Grubbs Pair ( $\alpha = 0.05$ )	---	---
Grubbs Pair ( $\alpha = 0.01$ )	---	---
Cochran ( $\alpha = 0.01$ )	---	---
Kolmogorov-Smirnov-Lilliefors Test	Distribution: normal	Distribution: normal

The outliers (Lab. 1, 1<sup>st</sup> run) was removed, the outliers (Lab. 11, 2<sup>nd</sup> run) was not removed.

Tab. 31: Outcome of statistical tests on the results obtained for Pb

	1 <sup>st</sup> run	2 <sup>nd</sup> run
Number of data sets	15	13
Scheffe's test (data compatible?)	yes	yes
Snedecor-F-Test and Bartlett-Test	Pooling not allowed	Pooling not allowed
Dixon ( $\alpha = 0.05$ )	Labs. 3 and 6	---
Dixon ( $\alpha = 0.01$ )	---	---
Nalimov ( $\alpha = 0.05$ )	Labs. 3 and 6	Lab. 2
Nalimov ( $\alpha = 0.01$ )	Lab. 6	---
Grubbs ( $\alpha = 0.05$ )	Lab. 6	---
Grubbs ( $\alpha = 0.01$ )	---	---
Grubbs Pair ( $\alpha = 0.05$ )	---	---
Grubbs Pair ( $\alpha = 0.01$ )	---	---
Cochran	Lab. 8	Lab. 8
Kolmogorov-Smirnov-Lilliefors Test	Distribution: normal	Distribution: normal

The outliers (Labs. 3 and 6, 1<sup>st</sup> run) were removed, the other outliers were not removed.

Tab. 32: Outcome of statistical tests on the results obtained for Mn

	1 <sup>st</sup> run	2 <sup>nd</sup> run
Number of data sets	13	12
Scheffe's test (data compatible?)	yes	yes
Snedecor-F-Test and Bartlett-Test	Pooling not allowed	Pooling not allowed
Dixon ( $\alpha = 0.05$ )	Lab. 11	---
Dixon ( $\alpha = 0.01$ )	---	---
Nalimov ( $\alpha = 0.05$ )	Lab. 11	Lab. 7
Nalimov ( $\alpha = 0.01$ )	Lab. 11	---
Grubbs ( $\alpha = 0.05$ )	Lab. 11	---
Grubbs ( $\alpha = 0.01$ )	---	---
Grubbs Pair ( $\alpha = 0.05$ )	---	---
Grubbs Pair ( $\alpha = 0.01$ )	---	---
Cochran	---	---
Kolmogorov-Smirnov-Lilliefors Test	Distribution: normal	Distribution: normal

The outlier (Lab. 11, 1<sup>st</sup> run) was removed.

Tab. 33: Outcome of statistical tests on the results obtained for Ni (“<-values” were not considered)

	1 <sup>st</sup> run	2 <sup>nd</sup> run
Number of data sets	14	13
Scheffe's test (data compatible?)	yes	yes
Snedecor-F-Test and Bartlett-Test	Pooling not allowed	Pooling not allowed
Dixon ( $\alpha = 0.05$ )	---	---
Dixon ( $\alpha = 0.01$ )	---	---
Nalimov ( $\alpha = 0.05$ )	Lab. 7	---
Nalimov ( $\alpha = 0.01$ )	Lab. 7	---
Grubbs ( $\alpha = 0.05$ )	Lab. 7	---
Grubbs ( $\alpha = 0.01$ )	---	---
Grubbs Pair ( $\alpha = 0.05$ )	---	---
Grubbs Pair ( $\alpha = 0.01$ )	---	---
Cochran	Lab. 8	Lab. 8
Kolmogorov-Smirnov-Lilliefors Test	Distribution: normal	Distribution: normal

The outlier (Lab. 7, 1<sup>st</sup> run) was removed, the other outliers were not removed.

Tab. 34: Outcome of statistical tests on the results obtained for Sb (“<-values” were not considered)

	1 <sup>st</sup> run	2 <sup>nd</sup> run
Number of data sets	12	11
Scheffe's test (data compatible?)	yes	yes
Snedecor-F-Test and Bartlett-Test	Pooling not allowed	Pooling not allowed
Dixon ( $\alpha = 0.05$ )	Lab. 6	---
Dixon ( $\alpha = 0.01$ )	Lab. 6	---
Nalimov ( $\alpha = 0.05$ )	Lab. 6	Lab. 2
Nalimov ( $\alpha = 0.01$ )	Lab. 6	---
Grubbs ( $\alpha = 0.05$ )	Lab. 6	---
Grubbs ( $\alpha = 0.01$ )	Lab. 6	---
Grubbs Pair ( $\alpha = 0.05$ )	---	---
Grubbs Pair ( $\alpha = 0.01$ )	---	---
Cochran	Lab. 13/I-2	Lab. 13/I-2
Kolmogorov-Smirnov-Lilliefors Test	Distribution: normal	Distribution: normal

The outlier (Lab. 6, 1<sup>st</sup> run) was removed, the other outliers were not removed.

Tab. 35: Outcome of statistical tests on the results obtained for S and Sn (“<-values” were not considered)

	S	Sn
Number of data sets	6	14
Scheffe's test (data compatible?)	yes	yes
Snedecor-F-Test and Bartlett-Test	Pooling not allowed	Pooling not allowed
Dixon ( $\alpha = 0.05$ )	---	---
Dixon ( $\alpha = 0.01$ )	---	---
Nalimov ( $\alpha = 0.05$ )	---	---
Nalimov ( $\alpha = 0.01$ )	---	---
Grubbs ( $\alpha = 0.05$ )	---	---
Grubbs ( $\alpha = 0.01$ )	---	---
Grubbs Pair ( $\alpha = 0.05$ )	---	---
Grubbs Pair ( $\alpha = 0.01$ )	---	---
Cochran	Lab. 11	Lab. 2
Kolmogorov-Smirnov-Lilliefors Test	Distribution: normal	Distribution: normal

The outliers were not removed.

Tab. 36: Outcome of statistical tests on the results obtained for Te (“<-values” were not considered)

	1 <sup>st</sup> run	2 <sup>nd</sup> run
Number of data sets	8	6
Scheffe's test (data compatible?)	yes	yes
Snedecor-F-Test and Bartlett-Test	Pooling not allowed	Pooling not allowed
Dixon ( $\alpha = 0.05$ )	---	---
Dixon ( $\alpha = 0.01$ )	---	---
Nalimov ( $\alpha = 0.05$ )	Lab. 7	---
Nalimov ( $\alpha = 0.01$ )	---	---
Grubbs ( $\alpha = 0.05$ )	---	---
Grubbs ( $\alpha = 0.01$ )	---	---
Grubbs Pair ( $\alpha = 0.05$ )	Labs. 5 and 7	---
Grubbs Pair ( $\alpha = 0.01$ )	Labs. 5 and 7	---
Cochran	---	---
Kolmogorov-Smirnov-Lilliefors Test	Distribution: normal	Distribution: normal

The outliers (Labs. 5 and 7) were removed.

Tab. 37: Outcome of statistical tests on the results obtained for Ti (“<-values” were not considered)

	Ti
Number of data sets	10
Scheffe's test (data compatible?)	yes
Snedecor-F-Test and Bartlett-Test	Pooling not allowed
Dixon ( $\alpha = 0.05$ )	---
Dixon ( $\alpha = 0.01$ )	---
Nalimov ( $\alpha = 0.05$ )	Lab. 11
Nalimov ( $\alpha = 0.01$ )	---
Grubbs ( $\alpha = 0.05$ )	---
Grubbs ( $\alpha = 0.01$ )	---
Grubbs Pair ( $\alpha = 0.05$ )	---
Grubbs Pair ( $\alpha = 0.01$ )	---
Cochran	---
Kolmogorov-Smirnov-Lilliefors Test	Distribution: normal

The outlier (Lab. 11) was not removed.

Tab. 38: Outcome of statistical tests on the results obtained for Zn

	1 <sup>st</sup> run	2 <sup>nd</sup> run
Number of data sets	9	8
Scheffe's test (data compatible?)	yes	yes
Snedecor-F-Test and Bartlett-Test	Pooling not allowed	Pooling not allowed
Dixon ( $\alpha = 0.05$ )	Lab. 7	---
Dixon ( $\alpha = 0.01$ )	---	---
Nalimov ( $\alpha = 0.05$ )	Lab. 7	Lab. 6
Nalimov ( $\alpha = 0.01$ )	Lab. 7	---
Grubbs ( $\alpha = 0.05$ )	Lab. 7	---
Grubbs ( $\alpha = 0.01$ )	---	---
Grubbs Pair ( $\alpha = 0.05$ )	---	---
Grubbs Pair ( $\alpha = 0.01$ )	---	---
Cochran	Lab. 6	Lab. 6
Kolmogorov-Smirnov-Lilliefors Test	Distribution: normal	Distribution: normal

The outlier (Lab. 7, 1<sup>st</sup> run) was removed, the other outliers were not removed.

The resp. combined uncertainties were calculated from the spread resulting from the certification inter-laboratory comparison ( $u_{ilc}$ ) and the uncertainty contributions from possible inhomogeneity of the material using Equation 1.

$$U_{\text{combined}} = \sqrt{u_{ilc}^2 + u_{bb}^2(1) + u_{bb}^2(2)} \quad (1)$$

with

$$u_{ilc} = \sqrt{\frac{s_M^2}{n}} : \text{uncertainty contribution resulting from inter-laboratory comparison}$$

$n$  : number of data sets used for calculating the certified mass fraction of each element

Table 39: Uncertainty calculation (uncertainty contribution from possible inhomogeneities  $u_{bb\_}(rel)$  estimated from the data of BAM-M384c for most of the elements)

	M	n	uncertainty contribution from				$u_{combined}$	$U$	$u_{bb\_}(rel)$	
			$s_M$	$u_{ilc}$	$u_{bb\_}(1)**$	$u_{bb\_}(2)**$			Length	Area
			mg/kg	mg/kg	mg/kg	mg/kg			mg/kg	mg/kg
Ag	10.20	13	0.3510	0.0974	0.0341	0.0401	0.1107	0.2214	0.3343	0.3935 **
As	1.20	13	0.1595	0.0442	0.0120	0.0240	0.0517	0.1035	1.0000	2.0000 ***
Bi	0.82	7	0.0689	0.0260	0.0085	0.0134	0.0305	0.0610	1.0350	1.6320 **
Cd	0.62	14	0.0601	0.0161	0.0127	0.0099	0.0227	0.0454	2.0450	1.5924 **
Co	1.30	14	0.0876	0.0234	0.0104	0.0118	0.0282	0.0565	0.8010	0.9112 **
Cr	0.77	12	0.1835	0.0530	0.0154	0.0179	0.0580	0.1160	2.0000	2.3243 ***
Fe	22.40	13	1.3468	0.3735	0.0792	0.1473	0.4093	0.8185	0.3534	0.6574 **
Mg	1.66	11	0.3041	0.0917	0.0167	0.0200	0.0953	0.1907	1.0086	1.2041 **
Mn	0.97	12	0.1310	0.0378	0.0098	0.0119	0.0408	0.0817	1.0132	1.2227 **
Ni	4.71	13	0.4447	0.1233	0.0701	0.1261	0.1898	0.3796	1.4881	2.6768 *
P	0.52	3	0.2151	0.1242	0.0104	0.0104	0.1250	0.2501	2.0000	2.0000 ***
Pb	7.75	13	1.4625	0.4056	0.1605	0.1655	0.4666	0.9331	2.0716	2.1349 **
S	3.48	6	0.6487	0.2648	0.0743	0.1010	0.2930	0.5860	2.1338	2.9020 **
Sb	1.78	11	0.2162	0.0652	0.0240	0.0387	0.0795	0.1590	1.3492	2.1756 **
Se	0.57	6	0.3738	0.1526	0.0114	0.0114	0.1534	0.3069	2.0000	2.0000 ***
Sn	3.81	15	0.4794	0.1238	0.0762	0.0762	0.1641	0.3282	2.0000	2.0000 ***
Te	0.47	6	0.0292	0.0119	0.0086	0.0161	0.0218	0.0437	1.8357	3.4284 **
Ti	1.18	10	0.3293	0.1041	0.0118	0.0236	0.1074	0.2149	1.0000	2.0000 ***
Zn	1.08	8	0.1585	0.0561	0.0189	0.0315	0.0670	0.1341	1.7544	2.9190 **

**calculated from $u_{bb\_}(rel)$ :	$u_{bb\_} = \frac{M \cdot u_{bb\_}(rel)}{100}$	*ext. Laboratory
		**BAM-M384c
		***estimated

The expanded uncertainties  $U$  are calculated by multiplication of  $u_{combined}$  with a coverage factor of  $k = 2$  using Equation 2.

$$U = k \cdot u_{combined} \quad (2)$$

The calculated mass fractions and their resp. expanded uncertainties are given on Page 3 of this report. Rounding was done according to DIN 1333 [4].

In addition to the wet chemical characterization some of the laboratories analysed the material with spark emission to check if there is agreement between SOES and wet chemistry. Tab. 40 shows the mean values of wet chemical and spark emission results as well as their standard deviations. The data obtained with wet chemistry and SOES are consistent for all elements except P, Sb, Te and Ti. It should be considered that for these elements there are only between three and four datasets obtained with SOES. The data from the spark emission inter-laboratory comparison was not used for the calculation of the certified values.

Tab. 40: Comparison wet chemistry vs. SOES

Element	Wet chemical analysis			Spark emission		
	Mass fraction in mg/kg	Std.-dev. in mg/kg	<i>n</i>	Mass fraction in mg/kg	Std.-dev. in mg/kg	<i>n</i>
Ag	10.2	0.4	13	10.1	0.6	5
As	1.20	0.16	13	1.24	0.12	3
Bi	0.82	0.07	7	0.87	0.18	5
Cd	0.62	0.06	14	0.95	0.26	3
Co	1.30	0.09	14	1.30	0.06	5
Cr	0.77	0.19	12	0.90	0.23	4
Fe	22.4	1.4	13	23.1	1.8	5
Mg	1.66	0.31	11	1.77	0.32	5
Mn	0.97	0.14	12	1.13	0.20	5
Ni	4.7	0.5	13	4.5	0.7	5
P	0.52	0.22	3	0.94	0.15	3
Pb	7.8	1.5	13	7.6	2.3	5
S	3.5	0.7	6	3.6	0.8	5
Sb	1.78	0.22	11	1.18	0.04	4
Se	0.57	0.37	6	0.63	0.19	2
Sn	3.8	0.5	15	3.9	0.2	4
Te	0.47	0.03	6	1.18	0.20	3
Ti	1.18	0.33	10	1.58	0.31	3
Zn	1.08	0.16	8	1.46	0.48	4
Zr	0.51	0.52	3	0.96	0.50	3

## 6. Instructions for users and stability statement

The certified reference material BAM-M383d is intended for the calibration and quality control of spark emission spectrometry used for the analysis of similar materials. It can also be used for wet chemical analysis.

Before analysis the surface of the material should be cleaned by turning or milling. The preparation of the surface has to be done slowly to avoid heating of the disc.

If chips prepared from the compact material are used for wet chemical analysis, a minimum sample intake of 0.2 g should be used.

The material will remain stable if it is not subjected to excessive heat (e.g., during preparation of the working surface).



## 7. Metrological Traceability

To ensure traceability of the certified mass fractions to the SI (Système International d'Unités) calibration was performed using standard solutions prepared from pure metals or stoichiometric compounds or traceable commercial calibration solutions.

## 8. References

- [1] DIN EN ISO 17034, General requirements for the competence of reference material producers, 2017
- [2] ISO Guide 31, Reference materials - Contents of certificates, labels and accompanying documentation, 2015
- [3] ISO Guide 35, Reference materials - Guidance for characterization and assessment of homogeneity and stability, 2017
- [4] DIN 1333:1992-02 Zahlenangaben

## 9. Information on and purchase of the CRM

Certified reference material BAM-M383d is supplied by  
**Bundesanstalt für Materialforschung und -prüfung (BAM)**  
Fachbereich 1.6: Anorganische Referenzmaterialien  
Richard-Willstätter-Str. 11, D-12489 Berlin, Germany  
Phone +49 (0)30 - 8104 2061  
Fax: +49 (0)30 - 8104 72061  
Email: [sales.crm@bam.de](mailto:sales.crm@bam.de)  
<https://www.webshop.bam.de>

Each disc will be distributed together with a detailed certificate containing the certified values and their uncertainties, the mean values and standard deviations of all accepted data sets and information on the analytical methods used and the names of the participating laboratories.

Information on certified reference materials can be obtained from BAM, <https://www.bam.de>.

**Annex 1:** Calculation of uncertainty contribution of potential inhomogeneity (length) ( $u_{bb}(\text{rel.})$ ) here means  $u_{bb}$  (rel) Length in Table 39), data from BAM-M384c

Ag in BAM-M384c

	1	2	3	4	5	
1.2e1	0.001484	0.001484	0.001470	0.001476	0.001548	
1.2a1	0.001486	0.001426	0.001442	0.001460	0.001487	
1.2a2	0.001512	0.001461	0.001444	0.001495	0.001519	
1.2a3	0.001469	0.001473	0.001419	0.001503	0.001530	
1.2e2	0.001509	0.001480	0.001438	0.001489	0.001519	
1.2e3	0.001497	0.001468	0.001442	0.001428	0.001468	
2.1a1	0.001486	0.001521	0.001472	0.001451	0.001459	
2.1a2	0.001518	0.001501	0.001455	0.001449	0.001464	
2.1a3	0.001532	0.001509	0.001424	0.001442	0.001478	
3.1e1	0.001526	0.001505	0.001489	0.001440	0.001462	
3.2e1	0.001514	0.001496	0.001467	0.001415	0.001441	
3.1e2	0.001518	0.001504	0.001459	0.001441	0.001467	
3.2e2	0.001521	0.001503	0.001460	0.001476	0.001478	
3.1e3	0.001535	0.001520	0.001482	0.001432	0.001474	
3.2e3	0.001515	0.001497	0.001466	0.001431	0.001473	
4.1e3	0.001522	0.001486	0.001412	0.001371	0.001457	
4.1e2	0.001518	0.001514	0.001471	0.001441	0.001468	
4.1e1	0.001529	0.001496	0.001470	0.001438	0.001456	
4.1a1	0.001523	0.001493	0.001494	0.001440	0.001481	
4.1a2	0.001522	0.001496	0.001487	0.001403	0.001466	
4.1a3	0.001534	0.001482	0.001478	0.001421	0.001489	
4.2a1	0.001519	0.001515	0.001478	0.001428	0.001464	
4.2a2	0.001523	0.001492	0.001474	0.001439	0.001458	
4.2a3	0.001503	0.001495	0.001497	0.001450	0.001457	
5.1a1	0.001538	0.001513	0.001473	0.001458	0.001500	
5.1a2	0.001535	0.001470	0.001474	0.001432	0.001452	
5.1a3	0.001505	0.001495	0.001473	0.001443	0.001457	
5.2a1	0.001515	0.001493	0.001472	0.001439	0.001462	
5.2a2	0.001504	0.001513	0.001477	0.001443	0.001486	
5.2a3	0.001503	0.001474	0.001463	0.001442	0.001471	
5.2e1	0.001519	0.001492	0.001461	0.001438	0.001487	
5.2e2	0.001532	0.001464	0.001456	0.001454	0.001488	
5.2e3	0.001510	0.001423	0.001464	0.001442	0.001460	
6.1e3	0.001524	0.001487	0.001479	0.001471	0.001462	
6.2e3	0.001530	0.001482	0.001430	0.001434	0.001489	
6.1e2	0.001525	0.001473	0.001469	0.001460	0.001457	
6.2e2	0.001516	0.001477	0.001475	0.001427	0.001462	
6.1e1	0.001556	0.001522	0.001491	0.001431	0.001496	
6.2e1	0.001551	0.001549	0.001439	0.001490	0.001537	
6.1a1	0.001493	0.001480	0.001426	0.001474	0.001509	
6.1a2	0.001509	0.001472	0.001466	0.001476	0.001527	
6.1a3	0.001493	0.001476	0.001454	0.001460	0.001528	
6.2a1	0.001502	0.001476	0.001430	0.001473	0.001494	
6.2a2	0.001499	0.001450	0.001440	0.001465	0.001521	
6.2a3	0.001494	0.001460	0.001475	0.001486	0.001507	
Source of variation	sums of squares (SS)	degrees of freedom (df)	Mean squares (MS)	F-value	P-value	critical F-value
Between group	2.52913E-08	44	5.74802E-10	0.4955199	0.9963892	1.4439497
Within groups	2.088E-07	180	1.16E-09			
Total	2.34091E-07	224				
within-sd	3.40587E-05					
effective n	5.00					
s <sub>bb</sub>	0					
s <sub>bb_min</sub>	4.94519E-06					
u <sub>bb</sub>	4.94519E-06					
u <sub>bb(rel.)</sub>	0.334320167					

Bi in BAM-M384c

	1	2	3	4	5	
1.2e1	0.000454	0.000464	0.000424	0.000476	0.000468	
1.2a1	0.000373	0.000422	0.000401	0.000426	0.000468	
1.2a2	0.000421	0.000415	0.000403	0.000431	0.000476	
1.2a3	0.000384	0.000401	0.000408	0.000438	0.000465	
1.2e2	0.000394	0.000421	0.000415	0.000450	0.000450	
1.2e3	0.000416	0.000381	0.000432	0.000405	0.000420	
2.1a1	0.000423	0.000424	0.000405	0.000407	0.000436	
2.1a2	0.000466	0.000396	0.000414	0.000405	0.000426	
2.1a3	0.000457	0.000400	0.000364	0.000406	0.000413	
3.1e1	0.000485	0.000394	0.000418	0.000427	0.000409	
3.2e1	0.000478	0.000423	0.000403	0.000434	0.000457	
3.1e2	0.000447	0.000383	0.000416	0.000363	0.000463	
3.2e2	0.000444	0.000393	0.000369	0.000448	0.000417	
3.1e3	0.000490	0.000393	0.000401	0.000407	0.000410	
3.2e3	0.000493	0.000414	0.000431	0.000411	0.000415	
4.1e3	0.000479	0.000394	0.000378	0.000390	0.000417	
4.1e2	0.000435	0.000417	0.000440	0.000419	0.000401	
4.1e1	0.000438	0.000397	0.000373	0.000427	0.000425	
4.1a1	0.000459	0.000417	0.000423	0.000422	0.000429	
4.1a2	0.000473	0.000391	0.000386	0.000391	0.000426	
4.1a3	0.000442	0.000403	0.000386	0.000404	0.000428	
4.2a1	0.000474	0.000397	0.000387	0.000410	0.000416	
4.2a2	0.000469	0.000388	0.000384	0.000394	0.000432	
4.2a3	0.000438	0.000384	0.000432	0.000404	0.000405	
5.1a1	0.000449	0.000414	0.000418	0.000450	0.000435	
5.1a2	0.000482	0.000389	0.000397	0.000402	0.000406	
5.1a3	0.000449	0.000398	0.000399	0.000383	0.000447	
5.2a1	0.000485	0.000401	0.000415	0.000397	0.000420	
5.2a2	0.000468	0.000402	0.000415	0.000422	0.000440	
5.2a3	0.000432	0.000407	0.000414	0.000431	0.000457	
5.2e1	0.000451	0.000395	0.000371	0.000400	0.000427	
5.2e2	0.000476	0.000416	0.000407	0.000408	0.000414	
5.2e3	0.000466	0.000350	0.000389	0.000432	0.000426	
6.1e3	0.000462	0.000375	0.000389	0.000409	0.000439	
6.2e3	0.000486	0.000435	0.000384	0.000415	0.000412	
6.1e2	0.000442	0.000418	0.000393	0.000394	0.000387	
6.2e2	0.000434	0.000433	0.000409	0.000360	0.000420	
6.1e1	0.000483	0.000420	0.000446	0.000470	0.000437	
6.2e1	0.000452	0.000533	0.000450	0.000420	0.000482	
6.1a1	0.000409	0.000405	0.000409	0.000447	0.000445	
6.1a2	0.000380	0.000379	0.000420	0.000439	0.000455	
6.1a3	0.000401	0.000402	0.000423	0.000440	0.000458	
6.2a1	0.000397	0.000418	0.000407	0.000428	0.000446	
6.2a2	0.000418	0.000420	0.000435	0.000412	0.000444	
6.2a3	0.000399	0.000400	0.000455	0.000455	0.000445	
Source of variation	sums of squares (SS)	degrees of freedom (df)	Mean squares (MS)	F-value	P-value	critical F-value
Between group	3.45235E-08	44	7.84626E-10	0.8655678	0.7082332	1.4439497
Within groups	1.63168E-07	180	9.06487E-10			
Total	1.97691E-07	224				
within-sd	3.01079E-05					
effective n	5.00					
s_bb	0					
s_bb_min	4.37155E-06					
u_bb	4.37155E-06					
u_bb(rel.)	1.034974024					

Cd in BAM-M384c

	1	2	3	4	5		
1.2e1	0.000455	0.000445	0.000430	0.000410	0.000379		
1.2a1	0.000413	0.000387	0.000364	0.000395	0.000390		
1.2a2	0.000439	0.000428	0.000405	0.000404	0.000380		
1.2a3	0.000428	0.000470	0.000413	0.000348	0.000387		
1.2e2	0.000423	0.000382	0.000439	0.000376	0.000414		
1.2e3	0.000408	0.000408	0.000409	0.000366	0.000426		
2.1a1	0.000441	0.000347	0.000444	0.000428	0.000399		
2.1a2	0.000460	0.000445	0.000429	0.000414	0.000424		
2.1a3	0.000428	0.000381	0.000454	0.000399	0.000421		
3.1e1	0.000439	0.000397	0.000425	0.000401	0.000376		
3.2e1	0.000447	0.000411	0.000408	0.000397	0.000404		
3.1e2	0.000468	0.000414	0.000413	0.000408	0.000408		
3.2e2	0.000463	0.000407	0.000411	0.000407	0.000418		
3.1e3	0.000402	0.000391	0.000450	0.000369	0.000387		
3.2e3	0.000382	0.000441	0.000387	0.000375	0.000380		
4.1e3	0.000469	0.000408	0.000404	0.000373	0.000397		
4.1e2	0.000435	0.000390	0.000376	0.000412	0.000423		
4.1e1	0.000420	0.000399	0.000374	0.000459	0.000421		
4.1a1	0.000450	0.000418	0.000417	0.000393	0.000400		
4.1a2	0.000466	0.000480	0.000458	0.000388	0.000407		
4.1a3	0.000451	0.000410	0.000415	0.000375	0.000412		
4.2a1	0.000434	0.000392	0.000424	0.000391	0.000416		
4.2a2	0.000432	0.000466	0.000397	0.000387	0.000400		
4.2a3	0.000415	0.000396	0.000414	0.000375	0.000423		
5.1a1	0.000460	0.000405	0.000436	0.000385	0.000424		
5.1a2	0.000413	0.000495	0.000437	0.000425	0.000430		
5.1a3	0.000398	0.000442	0.000403	0.000396	0.000405		
5.2a1	0.000425	0.000413	0.000412	0.000379	0.000412		
5.2a2	0.000434	0.000374	0.000380	0.000363	0.000395		
5.2a3	0.000414	0.000372	0.000397	0.000385	0.000394		
5.2e1	0.000440	0.000400	0.000477	0.000404	0.000397		
5.2e2	0.000439	0.000458	0.000387	0.000376	0.000363		
5.2e3	0.000408	0.000402	0.000384	0.000390	0.000382		
6.1e3	0.000427	0.000431	0.000444	0.000376	0.000393		
6.2e3	0.000402	0.000396	0.000420	0.000381	0.000402		
6.1e2	0.000416	0.000415	0.000425	0.000401	0.000392		
6.2e2	0.000389	0.000353	0.000407	0.000385	0.000387		
6.1e1	0.000388	0.000389	0.000390	0.000353	0.000392		
6.2e1	0.000436	0.000365	0.000394	0.000376	0.000391		
6.1a1	0.000396	0.000392	0.000367	0.000389	0.000362		
6.1a2	0.000389	0.000409	0.000368	0.000401	0.000393		
6.1a3	0.000431	0.000405	0.000358	0.000357	0.000362		
6.2a1	0.000448	0.000380	0.000397	0.000384	0.000377		
6.2a2	0.000460	0.000381	0.000392	0.000373	0.000391		
6.2a3	0.000400	0.000359	0.000382	0.000386	0.000409		
Source of variation	sums of squares (SS)	degrees of freedom (df)	Mean squares (MS)	F-value	P-value	critical F-value	
Between group	4.67726E-08	44	1.06301E-09	1.4822885	0.038956	1.4439497	
Within groups	1.29086E-07	180	7.17144E-10				
Total	1.75859E-07	224					
within-sd	2.67795E-05						
effective n	5.00						
s_bb	8.31709E-06						
s_bb_min	3.88828E-06						
u_bb	8.31709E-06						
u_bb(rel.)	2.045030528						

Co in BAM-M384c

	1	2	3	4	5	
1.2e1	0.000343	0.000352	0.000344	0.000373	0.000388	
1.2a1	0.000357	0.000340	0.000347	0.000358	0.000389	
1.2a2	0.000349	0.000339	0.000336	0.000358	0.000378	
1.2a3	0.000378	0.000340	0.000341	0.000356	0.000388	
1.2e2	0.000355	0.000346	0.000338	0.000359	0.000387	
1.2e3	0.000356	0.000344	0.000346	0.000349	0.000367	
2.1a1	0.000386	0.000366	0.000359	0.000345	0.000362	
2.1a2	0.000384	0.000365	0.000329	0.000336	0.000357	
2.1a3	0.000392	0.000377	0.000347	0.000341	0.000376	
3.1e1	0.000391	0.000352	0.000345	0.000353	0.000354	
3.2e1	0.000398	0.000361	0.000348	0.000341	0.000374	
3.1e2	0.000384	0.000355	0.000333	0.000332	0.000348	
3.2e2	0.000382	0.000367	0.000351	0.000336	0.000355	
3.1e3	0.000379	0.000361	0.000340	0.000348	0.000351	
3.2e3	0.000405	0.000356	0.000340	0.000338	0.000347	
4.1e3	0.000381	0.000364	0.000344	0.000350	0.000378	
4.1e2	0.000379	0.000380	0.000358	0.000349	0.000375	
4.1e1	0.000386	0.000350	0.000342	0.000339	0.000366	
4.1a1	0.000379	0.000386	0.000338	0.000341	0.000366	
4.1a2	0.000388	0.000351	0.000335	0.000344	0.000354	
4.1a3	0.000378	0.000360	0.000328	0.000335	0.000357	
4.2a1	0.000388	0.000369	0.000341	0.000337	0.000359	
4.2a2	0.000380	0.000379	0.000335	0.000340	0.000359	
4.2a3	0.000384	0.000342	0.000334	0.000338	0.000354	
5.1a1	0.000392	0.000362	0.000345	0.000348	0.000356	
5.1a2	0.000377	0.000377	0.000335	0.000337	0.000363	
5.1a3	0.000384	0.000372	0.000355	0.000338	0.000366	
5.2a1	0.000370	0.000366	0.000357	0.000332	0.000369	
5.2a2	0.000374	0.000353	0.000327	0.000347	0.000367	
5.2a3	0.000382	0.000382	0.000334	0.000347	0.000367	
5.2e1	0.000396	0.000357	0.000357	0.000325	0.000361	
5.2e2	0.000380	0.000381	0.000348	0.000337	0.000346	
5.2e3	0.000373	0.000374	0.000337	0.000346	0.000359	
6.1e3	0.000379	0.000370	0.000336	0.000342	0.000365	
6.2e3	0.000377	0.000355	0.000359	0.000332	0.000349	
6.1e2	0.000384	0.000376	0.000349	0.000339	0.000352	
6.2e2	0.000382	0.000388	0.000354	0.000343	0.000360	
6.1e1	0.000397	0.000357	0.000335	0.000340	0.000374	
6.2e1	0.000355	0.000348	0.000339	0.000366	0.000385	
6.1a1	0.000360	0.000331	0.000343	0.000363	0.000397	
6.1a2	0.000361	0.000332	0.000340	0.000355	0.000390	
6.1a3	0.000368	0.000339	0.000339	0.000370	0.000383	
6.2a1	0.000370	0.000358	0.000347	0.000360	0.000393	
6.2a2	0.000383	0.000348	0.000336	0.000348	0.000391	
6.2a3	0.000360	0.000336	0.000363	0.000371	0.000387	
Source of variation	sums of squares (SS)	degrees of freedom (df)	Mean squares (MS)	F-value	P-value	critical F-value
Between group	3.98089E-09	44	9.04747E-11	0.2308684	0.9999999	1.4439497
Within groups	7.054E-08	180	3.91889E-10			
Total	7.45209E-08	224				
within-sd	1.97962E-05					
effective n	5.00					
s_bb	0					
s_bb_min	2.87432E-06					
u_bb	2.87432E-06					
u_bb(rel.)	0.801044262					

Fe in BAM-M384c

	1	2	3	4	5	
1.2e1	0.003597	0.003653	0.003626	0.003770	0.003777	
1.2a1	0.003731	0.003615	0.003651	0.003803	0.003744	
1.2a2	0.003696	0.003578	0.003570	0.003695	0.003708	
1.2a3	0.003689	0.003573	0.003672	0.003758	0.003796	
1.2e2	0.003692	0.003631	0.003638	0.003748	0.003785	
1.2e3	0.003635	0.003603	0.003655	0.003637	0.003737	
2.1a1	0.003782	0.003686	0.003668	0.003597	0.003686	
2.1a2	0.003747	0.003701	0.003601	0.003634	0.003762	
2.1a3	0.003819	0.003748	0.003689	0.003632	0.003809	
3.1e1	0.003833	0.003665	0.003629	0.003708	0.003774	
3.2e1	0.004228	0.003686	0.003631	0.003663	0.003810	
3.1e2	0.003826	0.003679	0.003619	0.003587	0.003714	
3.2e2	0.003777	0.003662	0.003581	0.003606	0.003702	
3.1e3	0.003716	0.003693	0.003595	0.003697	0.003675	
3.2e3	0.003848	0.003631	0.003615	0.003624	0.003856	
4.1e3	0.003731	0.003722	0.003594	0.003660	0.003829	
4.1e2	0.003783	0.003739	0.003682	0.003690	0.003811	
4.1e1	0.003775	0.003639	0.003597	0.003644	0.003737	
4.1a1	0.003735	0.003708	0.003563	0.003652	0.003702	
4.1a2	0.003799	0.003680	0.003604	0.003652	0.003734	
4.1a3	0.003779	0.003692	0.003576	0.003606	0.003716	
4.2a1	0.003769	0.003730	0.003627	0.003685	0.003811	
4.2a2	0.003758	0.003760	0.003568	0.003623	0.003718	
4.2a3	0.003773	0.003630	0.003600	0.003604	0.003729	
5.1a1	0.003844	0.003652	0.003686	0.003627	0.003729	
5.1a2	0.003729	0.003693	0.003531	0.003614	0.003710	
5.1a3	0.003767	0.003791	0.003766	0.003625	0.003767	
5.2a1	0.003673	0.003688	0.003669	0.003612	0.003829	
5.2a2	0.003714	0.003651	0.003507	0.003687	0.003769	
5.2a3	0.003719	0.003724	0.003623	0.003608	0.003777	
5.2e1	0.003782	0.003621	0.003687	0.003584	0.003736	
5.2e2	0.003734	0.003745	0.003752	0.003645	0.003715	
5.2e3	0.003766	0.003781	0.003572	0.003686	0.003754	
6.1e3	0.003783	0.003712	0.003576	0.003620	0.003775	
6.2e3	0.003887	0.003667	0.003776	0.003579	0.003710	
6.1e2	0.003823	0.003759	0.003611	0.003616	0.003690	
6.2e2	0.003778	0.003740	0.003664	0.003604	0.003702	
6.1e1	0.003809	0.003671	0.003547	0.003620	0.003760	
6.2e1	0.003671	0.003618	0.003661	0.003746	0.003752	
6.1a1	0.003673	0.003578	0.003651	0.003837	0.003803	
6.1a2	0.003683	0.003531	0.003634	0.003763	0.003789	
6.1a3	0.003793	0.003557	0.003600	0.003796	0.003780	
6.2a1	0.003755	0.003725	0.003694	0.003786	0.003848	
6.2a2	0.003738	0.003652	0.003559	0.003676	0.003821	
6.2a3	0.003674	0.003594	0.003772	0.003816	0.003829	
Source of variation	sums of squares (SS)	degrees of freedom (df)	Mean squares (MS)	F-value	P-value	critical F-value
Between group	1.9423E-07	44	4.41433E-09	0.5446688	0.9904162	1.4439497
Within groups	1.45883E-06	180	8.10461E-09			
Total	1.65306E-06	224				
within-sd	9.00256E-05					
effective n	5.00					
s_bb	0					
s_bb_min	1.30713E-05					
u_bb	1.30713E-05					
u_bb(rel.)	0.35338794					

Mg in BAM-M384c

	1	2	3	4	5	
1.2e1	0.000281	0.000309	0.000327	0.000298	0.000313	
1.2a1	0.000304	0.000296	0.000321	0.000295	0.000326	
1.2a2	0.000285	0.000288	0.000308	0.000290	0.000304	
1.2a3	0.000265	0.000275	0.000314	0.000288	0.000297	
1.2e2	0.000273	0.000286	0.000313	0.000295	0.000316	
1.2e3	0.000279	0.000287	0.000318	0.000284	0.000308	
2.1a1	0.000277	0.000279	0.000310	0.000285	0.000286	
2.1a2	0.000269	0.000282	0.000297	0.000287	0.000292	
2.1a3	0.000268	0.000281	0.000293	0.000276	0.000297	
3.1e1	0.000282	0.000289	0.000312	0.000290	0.000311	
3.2e1	0.000275	0.000284	0.000309	0.000288	0.000305	
3.1e2	0.000275	0.000286	0.000311	0.000290	0.000308	
3.2e2	0.000289	0.000292	0.000315	0.000286	0.000302	
3.1e3	0.000285	0.000282	0.000306	0.000297	0.000307	
3.2e3	0.000285	0.000289	0.000315	0.000288	0.000305	
4.1e3	0.000289	0.000296	0.000324	0.000307	0.000316	
4.1e2	0.000293	0.000313	0.000336	0.000309	0.000321	
4.1e1	0.000297	0.000294	0.000328	0.000302	0.000326	
4.1a1	0.000288	0.000302	0.000331	0.000300	0.000327	
4.1a2	0.000294	0.000323	0.000323	0.000304	0.000325	
4.1a3	0.000282	0.000291	0.000324	0.000298	0.000316	
4.2a1	0.000289	0.000282	0.000331	0.000300	0.000310	
4.2a2	0.000287	0.000300	0.000314	0.000291	0.000308	
4.2a3	0.000284	0.000285	0.000316	0.000300	0.000305	
5.1a1	0.000292	0.000308	0.000316	0.000293	0.000323	
5.1a2	0.000308	0.000292	0.000294	0.000322	0.000316	
5.1a3	0.000286	0.000307	0.000326	0.000300	0.000310	
5.2a1	0.000285	0.000283	0.000315	0.000292	0.000314	
5.2a2	0.000284	0.000284	0.000314	0.000293	0.000305	
5.2a3	0.000286	0.000288	0.000310	0.000288	0.000299	
5.2e1	0.000281	0.000293	0.000310	0.000310	0.000318	
5.2e2	0.000289	0.000306	0.000318	0.000297	0.000320	
5.2e3	0.000282	0.000291	0.000328	0.000300	0.000315	
6.1e3	0.000298	0.000299	0.000321	0.000299	0.000314	
6.2e3	0.000297	0.000301	0.000317	0.000290	0.000317	
6.1e2	0.000281	0.000289	0.000319	0.000306	0.000305	
6.2e2	0.000286	0.000284	0.000319	0.000287	0.000329	
6.1e1	0.000295	0.000323	0.000323	0.000304	0.000327	
6.2e1	0.000291	0.000302	0.000318	0.000303	0.000312	
6.1a1	0.000307	0.000279	0.000296	0.000315	0.000288	
6.1a2	0.000286	0.000293	0.000317	0.000297	0.000317	
6.1a3	0.000279	0.000297	0.000320	0.000299	0.000316	
6.2a1	0.000290	0.000290	0.000315	0.000303	0.000312	
6.2a2	0.000295	0.000298	0.000322	0.000293	0.000313	
6.2a3	0.000286	0.000285	0.000322	0.000306	0.000307	
Source of variation	sums of squares (SS)	degrees of freedom (df)	Mean squares (MS)	F-value	P-value	critical F-value
Between group	1.14625E-08	44	2.60511E-10	1.2143376	0.1898828	1.4439497
Within groups	3.86152E-08	180	2.14529E-10			
Total	5.00777E-08	224				
within-sd	1.46468E-05					
effective n	5.00					
s_bb	3.03254E-06					
s_bb_min	2.12666E-06					
u_bb	3.03254E-06					
u_bb(rel.)	1.00859175					

Mn in BAM-M384c

	1	2	3	4	5	
1.2e1	0.000861	0.001006	0.000969	0.000868	0.000901	
1.2a1	0.000887	0.000868	0.001018	0.000864	0.000903	
1.2a2	0.000894	0.000913	0.000940	0.000798	0.000932	
1.2a3	0.000920	0.000887	0.000993	0.000811	0.000910	
1.2e2	0.000874	0.000885	0.000976	0.000861	0.000887	
1.2e3	0.000869	0.000922	0.001004	0.000998	0.000874	
2.1a1	0.000907	0.000874	0.000998	0.000978	0.000858	
2.1a2	0.000903	0.000902	0.000918	0.000947	0.000836	
2.1a3	0.000906	0.000879	0.000901	0.001056	0.000824	
3.1e1	0.000869	0.000870	0.000904	0.001049	0.000809	
3.2e1	0.000944	0.000897	0.000939	0.001031	0.000880	
3.1e2	0.000920	0.000886	0.001004	0.000922	0.000856	
3.2e2	0.000855	0.000849	0.000881	0.000932	0.000800	
3.1e3	0.000905	0.000851	0.000847	0.001023	0.000813	
3.2e3	0.000955	0.000887	0.000998	0.001023	0.000846	
4.1e3	0.000894	0.000882	0.000856	0.000940	0.000892	
4.1e2	0.000906	0.000929	0.000993	0.001026	0.000869	
4.1e1	0.000922	0.000864	0.000859	0.000953	0.000883	
4.1a1	0.000894	0.000925	0.000869	0.000987	0.000825	
4.1a2	0.000953	0.000834	0.000840	0.000910	0.000837	
4.1a3	0.000915	0.000896	0.000825	0.000890	0.000835	
4.2a1	0.000912	0.000853	0.000905	0.000979	0.000865	
4.2a2	0.000896	0.000971	0.000892	0.000947	0.000854	
4.2a3	0.000941	0.000837	0.000833	0.000937	0.000860	
5.1a1	0.000898	0.000847	0.000896	0.000999	0.000791	
5.1a2	0.000887	0.000903	0.000873	0.000971	0.000860	
5.1a3	0.000905	0.000881	0.000957	0.000974	0.000848	
5.2a1	0.000900	0.000932	0.000947	0.000966	0.000920	
5.2a2	0.000914	0.000817	0.000896	0.001041	0.000802	
5.2a3	0.000880	0.000980	0.000949	0.001002	0.000870	
5.2e1	0.000929	0.000887	0.001011	0.000945	0.000818	
5.2e2	0.000894	0.000887	0.000904	0.000929	0.000766	
5.2e3	0.000883	0.000766	0.000862	0.000993	0.000836	
6.1e3	0.000891	0.000878	0.000880	0.000917	0.000836	
6.2e3	0.000860	0.000918	0.000984	0.000933	0.000747	
6.1e2	0.000897	0.001009	0.000900	0.000948	0.000849	
6.2e2	0.000908	0.001049	0.000879	0.001017	0.000831	
6.1e1	0.000919	0.000841	0.000879	0.000892	0.000809	
6.2e1	0.000845	0.000849	0.000982	0.000810	0.000788	
6.1a1	0.000858	0.000883	0.000956	0.000802	0.000930	
6.1a2	0.000860	0.000896	0.000911	0.000857	0.000915	
6.1a3	0.000878	0.000858	0.000998	0.000848	0.000860	
6.2a1	0.000871	0.000906	0.001034	0.000845	0.000903	
6.2a2	0.000939	0.000995	0.000964	0.000861	0.000886	
6.2a3	0.000829	0.000871	0.001042	0.000904	0.000951	
Source of variation	sums of squares (SS)	degrees of freedom (df)	Mean squares (MS)	F-value	P-value	critical F-value
Between group	1.14796E-07	44	2.609E-09	0.6577187	0.9488385	1.4439497
Within groups	7.14014E-07	180	3.96675E-09			
Total	8.28811E-07	224				
within-sd	6.29821E-05					
effective n	5.00					
s_bb	0					
s_bb_min	9.14475E-06					
u_bb	9.14475E-06					
u_bb(rel.)	1.013170858					



Ni in BAM-M384c

	1	2	3	4	5	
1.2e1	0.000608	0.000778	0.000718	0.000637	0.000831	
1.2a1	0.000675	0.000701	0.000709	0.000597	0.000750	
1.2a2	0.000585	0.000671	0.000726	0.000614	0.000723	
1.2a3	0.000650	0.000700	0.000661	0.000609	0.000760	
1.2e2	0.000564	0.000698	0.000656	0.000620	0.000774	
1.2e3	0.000753	0.000706	0.000707	0.000614	0.000789	
2.1a1	0.000661	0.000696	0.000690	0.000633	0.000733	
2.1a2	0.000583	0.000695	0.000701	0.000739	0.000704	
2.1a3	0.000574	0.000654	0.000684	0.000644	0.000774	
3.1e1	0.000602	0.000747	0.000655	0.000609	0.000839	
3.2e1	0.000641	0.000650	0.000667	0.000662	0.000776	
3.1e2	0.000617	0.000631	0.000696	0.000645	0.000791	
3.2e2	0.000747	0.000791	0.000655	0.000610	0.000791	
3.1e3	0.000584	0.000675	0.000645	0.000579	0.000718	
3.2e3	0.000568	0.000725	0.000662	0.000588	0.000809	
4.1e3	0.000584	0.000742	0.000660	0.000598	0.000763	
4.1e2	0.000554	0.000734	0.000695	0.000628	0.000713	
4.1e1	0.000569	0.000703	0.000701	0.000674	0.000795	
4.1a1	0.000587	0.000725	0.000691	0.000644	0.000746	
4.1a2	0.000635	0.000719	0.000698	0.000588	0.000774	
4.1a3	0.000555	0.000658	0.000792	0.000711	0.000697	
4.2a1	0.000575	0.000715	0.000654	0.000586	0.000747	
4.2a2	0.000620	0.000740	0.000675	0.000693	0.000713	
4.2a3	0.000625	0.000650	0.000634	0.000618	0.000756	
5.1a1	0.000618	0.000678	0.000684	0.000607	0.000803	
5.1a2	0.000654	0.000715	0.000619	0.000708	0.000701	
5.1a3	0.000617	0.000758	0.000677	0.000609	0.000738	
5.2a1	0.000591	0.000739	0.000623	0.000592	0.000725	
5.2a2	0.000606	0.000732	0.000666	0.000597	0.000718	
5.2a3	0.000592	0.000637	0.000638	0.000593	0.000745	
5.2e1	0.000638	0.000681	0.000678	0.000753	0.000745	
5.2e2	0.000609	0.000763	0.000695	0.000621	0.000712	
5.2e3	0.000601	0.000682	0.000708	0.000587	0.000718	
6.1e3	0.000593	0.000721	0.000691	0.000639	0.000773	
6.2e3	0.000579	0.000758	0.000612	0.000652	0.000801	
6.1e2	0.000717	0.000674	0.000723	0.000717	0.000626	
6.2e2	0.000592	0.000676	0.000700	0.000606	0.000830	
6.1e1	0.000601	0.000688	0.000670	0.000622	0.000770	
6.2e1	0.000622	0.000737	0.000674	0.000597	0.000686	
6.1a1	0.000737	0.000594	0.000727	0.000648	0.000635	
6.1a2	0.000585	0.000664	0.000624	0.000614	0.000714	
6.1a3	0.000592	0.000729	0.000625	0.000690	0.000740	
6.2a1	0.000663	0.000650	0.000693	0.000622	0.000809	
6.2a2	0.000689	0.000673	0.000699	0.000631	0.000723	
6.2a3	0.000553	0.000690	0.000669	0.000561	0.000714	
Source of variation	sums of squares (SS)	degrees of freedom (df)	Mean squares (MS)	F-value	P-value	critical F-value
Between group	7.26246E-08	44	1.65056E-09	0.344626	0.9999595	1.4439497
Within groups	8.62096E-07	180	4.78942E-09			
Total	9.34721E-07	224				
within-sd	6.92057E-05					
effective n	5.00					
s_bb	0					
s_bb_min	1.00484E-05					
u_bb	1.00484E-05					
u_bb(rel.)	1.488080544					

Pb in BAM-M384c

1.2e1	0.000967	0.001117	0.001062	0.001117	0.001233	
1.2a1	0.001069	0.000984	0.001017	0.000946	0.001348	
1.2a2	0.000982	0.000950	0.001044	0.001068	0.001242	
1.2a3	0.000985	0.001241	0.001075	0.000969	0.001198	
1.2e2	0.000959	0.000899	0.001039	0.001255	0.001282	
1.2e3	0.000946	0.000980	0.001109	0.000978	0.001254	
2.1a1	0.000928	0.000841	0.000976	0.000992	0.001214	
2.1a2	0.000890	0.000887	0.000991	0.001039	0.001190	
2.1a3	0.000961	0.000904	0.001058	0.001044	0.001237	
3.1e1	0.000878	0.000831	0.000971	0.000922	0.001256	
3.2e1	0.000915	0.000890	0.000997	0.000991	0.001207	
3.1e2	0.000954	0.000836	0.001042	0.000916	0.001270	
3.2e2	0.000961	0.001034	0.001025	0.001023	0.001166	
3.1e3	0.000907	0.000826	0.000957	0.000919	0.001156	
3.2e3	0.001059	0.001100	0.001102	0.001115	0.001261	
4.1e3	0.000959	0.001083	0.001000	0.001071	0.001266	
4.1e2	0.001032	0.000907	0.001028	0.001193	0.001304	
4.1e1	0.000959	0.000986	0.001063	0.001049	0.001308	
4.1a1	0.000966	0.001031	0.001056	0.001057	0.001232	
4.1a2	0.001031	0.000982	0.001042	0.000974	0.001255	
4.1a3	0.001046	0.000835	0.001180	0.001073	0.001217	
4.2a1	0.000931	0.000870	0.001057	0.000993	0.001231	
4.2a2	0.000909	0.000987	0.001041	0.001051	0.001193	
4.2a3	0.000935	0.000874	0.001009	0.001137	0.001456	
5.1a1	0.000936	0.000778	0.000891	0.000929	0.001210	
5.1a2	0.000874	0.000974	0.000752	0.001032	0.001152	
5.1a3	0.000807	0.000901	0.001708	0.000904	0.001069	
5.2a1	0.000911	0.000844	0.000867	0.000862	0.001197	
5.2a2	0.000880	0.001029	0.000905	0.000913	0.001157	
5.2a3	0.000925	0.000774	0.000904	0.000850	0.001199	
5.2e1	0.000844	0.000833	0.000942	0.001011	0.001151	
5.2e2	0.000954	0.000940	0.001010	0.000970	0.001333	
5.2e3	0.000856	0.000840	0.001003	0.000970	0.001111	
6.1e3	0.000922	0.000833	0.001008	0.001021	0.001226	
6.2e3	0.000914	0.001044	0.000882	0.001032	0.001195	
6.1e2	0.000837	0.000841	0.000924	0.000928	0.001158	
6.2e2	0.000962	0.000826	0.001010	0.000937	0.001263	
6.1e1	0.000905	0.000830	0.001015	0.001014	0.000982	
6.2e1	0.000949	0.000965	0.000983	0.000928	0.001158	
6.1a1	0.001345	0.000906	0.000984	0.001000	0.000946	
6.1a2	0.000832	0.000822	0.000895	0.000932	0.001241	
6.1a3	0.000958	0.000934	0.000897	0.000992	0.001166	
6.2a1	0.000982	0.000848	0.000996	0.000941	0.001211	
6.2a2	0.001072	0.000935	0.001113	0.000971	0.001237	
6.2a3	0.000956	0.000927	0.001012	0.000960	0.001166	
Source of variation	sums of squares (SS)	degrees of freedom (df)	Mean squares (MS)	F-value	P-value	critical F-value
Between group	6.25921E-07	44	1.42255E-08	0.6723745	0.939303	1.4439497
Within groups	3.80827E-06	180	2.11571E-08			
Total	4.43419E-06	224				
within-sd	0.000145455					
effective n	5.00					
s_bb	0					
s_bb_min	2.11194E-05					
u_bb	2.11194E-05					
u_bb(rel.)	2.071579299					

S in BAM-M384c

	1	2	3	4	5	
1.2e1	0.000431	0.000340	0.000414	0.000335	0.000333	
1.2a1	0.000308	0.000325	0.000271	0.000315	0.000240	
1.2a2	0.000295	0.000323	0.000447	0.000314	0.000366	
1.2a3	0.000324	0.000403	0.000365	0.000254	0.000331	
1.2e2	0.000312	0.000285	0.000445	0.000383	0.000327	
1.2e3	0.000354	0.000386	0.000409	0.000300	0.000396	
2.1a1	0.000452	0.000297	0.000399	0.000369	0.000247	
2.1a2	0.000291	0.000306	0.000388	0.000375	0.000307	
2.1a3	0.000282	0.000316	0.000365	0.000306	0.000342	
3.1e1	0.000291	0.000368	0.000321	0.000317	0.000358	
3.2e1	0.000307	0.000279	0.000379	0.000317	0.000323	
3.1e2	0.000340	0.000293	0.000394	0.000342	0.000290	
3.2e2	0.000383	0.000462	0.000337	0.000336	0.000324	
3.1e3	0.000293	0.000325	0.000400	0.000327	0.000209	
3.2e3	0.000251	0.000372	0.000402	0.000362	0.000294	
4.1e3	0.000311	0.000316	0.000397	0.000362	0.000355	
4.1e2	0.000265	0.000311	0.000371	0.000274	0.000270	
4.1e1	0.000232	0.000296	0.000380	0.000370	0.000293	
4.1a1	0.000267	0.000285	0.000317	0.000346	0.000221	
4.1a2	0.000302	0.000410	0.000453	0.000285	0.000305	
4.1a3	0.000271	0.000293	0.000390	0.000315	0.000283	
4.2a1	0.000276	0.000333	0.000331	0.000339	0.000323	
4.2a2	0.000285	0.000341	0.000340	0.000377	0.000302	
4.2a3	0.000332	0.000369	0.000378	0.000302	0.000286	
5.1a1	0.000319	0.000323	0.000361	0.000296	0.000277	
5.1a2	0.000316	0.000423	0.000304	0.000413	0.000315	
5.1a3	0.000297	0.000307	0.000298	0.000346	0.000323	
5.2a1	0.000253	0.000380	0.000367	0.000316	0.000285	
5.2a2	0.000335	0.000341	0.000343	0.000316	0.000281	
5.2a3	0.000243	0.000306	0.000354	0.000403	0.000309	
5.2e1	0.000308	0.000301	0.000396	0.000438	0.000287	
5.2e2	0.000274	0.000337	0.000340	0.000345	0.000332	
5.2e3	0.000354	0.000324	0.000328	0.000327	0.000291	
6.1e3	0.000336	0.000406	0.000337	0.000247	0.000299	
6.2e3	0.000264	0.000301	0.000377	0.000278	0.000358	
6.1e2	0.000292	0.000294	0.000428	0.000332	0.000293	
6.2e2	0.000270	0.000327	0.000316	0.000362	0.000319	
6.1e1	0.000392	0.000313	0.000359	0.000372	0.000286	
6.2e1	0.000264	0.000321	0.000410	0.000350	0.000358	
6.1a1	0.000280	0.000283	0.000319	0.000371	0.000326	
6.1a2	0.000321	0.000293	0.000378	0.000302	0.000281	
6.1a3	0.000311	0.000276	0.000317	0.000334	0.000243	
6.2a1	0.000384	0.000299	0.000335	0.000322	0.000288	
6.2a2	0.000318	0.000266	0.000387	0.000338	0.000253	
6.2a3	0.000303	0.000320	0.000365	0.000313	0.000325	
Source of variation	sums of squares (SS)	degrees of freedom (df)	Mean squares (MS)	F-value	P-value	critical F-value
Between group	8.18657E-08	44	1.86058E-09	0.7991522	0.8079658	1.4439497
Within groups	4.19076E-07	180	2.3282E-09			
Total	5.00941E-07	224				
within-sd	4.82514E-05					
effective n	5.00					
s_bb	0					
s_bb_min	7.00591E-06					
u_bb	7.00591E-06					
u_bb(rel.)	2.133836244					

Sb in BAM-M384c

	1	2	3	4	5	
1.2e1	0.000981	0.000999	0.000881	0.000889	0.001020	
1.2a1	0.000857	0.000835	0.000766	0.000881	0.000996	
1.2a2	0.000881	0.000841	0.000897	0.000830	0.000991	
1.2a3	0.000896	0.000756	0.000702	0.000890	0.001019	
1.2e2	0.000814	0.000750	0.000907	0.001034	0.000871	
1.2e3	0.000988	0.000835	0.000783	0.000771	0.000760	
2.1a1	0.000884	0.000949	0.000866	0.000881	0.000804	
2.1a2	0.000928	0.000812	0.000891	0.000815	0.000813	
2.1a3	0.000959	0.000816	0.000807	0.000861	0.000847	
3.1e1	0.000974	0.000897	0.000770	0.000718	0.000889	
3.2e1	0.001018	0.000843	0.000800	0.000746	0.000965	
3.1e2	0.000991	0.000850	0.000958	0.000826	0.000931	
3.2e2	0.000943	0.000921	0.000856	0.000852	0.000968	
3.1e3	0.000957	0.000903	0.000809	0.000763	0.000795	
3.2e3	0.001024	0.001027	0.000873	0.000833	0.000870	
4.1e3	0.000997	0.000917	0.000788	0.000701	0.000903	
4.1e2	0.001034	0.000846	0.000892	0.000883	0.000898	
4.1e1	0.000981	0.000856	0.000815	0.000859	0.000852	
4.1a1	0.001045	0.000896	0.000813	0.000779	0.000879	
4.1a2	0.000964	0.000763	0.000818	0.000796	0.001031	
4.1a3	0.001004	0.000851	0.000834	0.000833	0.000883	
4.2a1	0.001013	0.000903	0.000783	0.000843	0.000819	
4.2a2	0.000948	0.000856	0.000803	0.000767	0.000810	
4.2a3	0.000941	0.000791	0.000861	0.000810	0.000837	
5.1a1	0.000907	0.000990	0.000882	0.000870	0.000823	
5.1a2	0.001015	0.000801	0.000830	0.000790	0.000797	
5.1a3	0.000889	0.000968	0.000843	0.000791	0.000764	
5.2a1	0.001061	0.000851	0.000948	0.000817	0.000858	
5.2a2	0.000941	0.000800	0.000809	0.000830	0.000832	
5.2a3	0.000811	0.000833	0.000923	0.000807	0.000811	
5.2e1	0.000895	0.000910	0.000883	0.000747	0.000850	
5.2e2	0.000963	0.000855	0.000811	0.000753	0.000821	
5.2e3	0.000941	0.000750	0.000730	0.000809	0.000792	
6.1e3	0.000918	0.000793	0.000794	0.000863	0.000807	
6.2e3	0.000960	0.001005	0.000879	0.000862	0.000782	
6.1e2	0.001003	0.000898	0.000845	0.000820	0.000865	
6.2e2	0.000898	0.000947	0.000805	0.000830	0.000802	
6.1e1	0.000947	0.000939	0.000840	0.000967	0.000933	
6.2e1	0.000946	0.001028	0.000911	0.000804	0.001005	
6.1a1	0.000946	0.000739	0.000818	0.000972	0.000909	
6.1a2	0.000804	0.000849	0.000883	0.000935	0.000947	
6.1a3	0.000784	0.000757	0.000870	0.000879	0.001006	
6.2a1	0.000804	0.000831	0.000812	0.000926	0.000916	
6.2a2	0.000962	0.000885	0.000916	0.000869	0.000945	
6.2a3	0.000856	0.000747	0.000867	0.000885	0.001044	
Source of variation	sums of squares (SS)	degrees of freedom (df)	Mean squares (MS)	F-value	P-value	critical F-value
Between group	2.1689E-07	44	4.92932E-09	0.7486412	0.8707373	1.4439497
Within groups	1.18518E-06	180	6.58436E-09			
Total	1.40207E-06	224				
within-sd	8.1144E-05					
effective n	5.00					
s_bb	0					
s_bb_min	1.17818E-05					
u_bb	1.17818E-05					
u_bb(rel.)	1.349189542					

Te in BAM-M384c

	1	2	3	4	5	
1.2e1	0.000720	0.000885	0.000597	0.000727	0.000712	
1.2a1	0.000649	0.000678	0.000556	0.000817	0.000782	
1.2a2	0.000785	0.000533	0.000625	0.000684	0.000738	
1.2a3	0.000559	0.000647	0.000655	0.000677	0.000794	
1.2e2	0.000805	0.000609	0.000663	0.000635	0.000726	
1.2e3	0.000849	0.000575	0.000709	0.000620	0.000641	
2.1a1	0.000757	0.000616	0.000639	0.000620	0.000598	
2.1a2	0.000632	0.000661	0.000691	0.000647	0.000642	
2.1a3	0.000835	0.000684	0.000562	0.000609	0.000760	
3.1e1	0.000842	0.000823	0.000666	0.000677	0.000698	
3.2e1	0.000704	0.000708	0.000578	0.000625	0.000625	
3.1e2	0.000767	0.000652	0.000759	0.000634	0.000760	
3.2e2	0.000774	0.000639	0.000595	0.000660	0.000697	
3.1e3	0.000908	0.000614	0.000560	0.000759	0.000768	
3.2e3	0.000832	0.000754	0.000651	0.000549	0.000597	
4.1e3	0.000703	0.000616	0.000610	0.000591	0.000757	
4.1e2	0.000776	0.000667	0.000744	0.000577	0.000735	
4.1e1	0.000623	0.000650	0.000687	0.000635	0.000664	
4.1a1	0.000646	0.000660	0.000632	0.000632	0.000724	
4.1a2	0.000641	0.000595	0.000595	0.000642	0.000860	
4.1a3	0.000744	0.000743	0.000612	0.000596	0.000677	
4.2a1	0.000678	0.000669	0.000707	0.000743	0.000602	
4.2a2	0.000736	0.000601	0.000469	0.000657	0.000609	
4.2a3	0.000715	0.000687	0.000793	0.000663	0.000720	
5.1a1	0.000722	0.000815	0.000701	0.000672	0.000692	
5.1a2	0.000899	0.000728	0.000774	0.000592	0.000754	
5.1a3	0.000767	0.000590	0.000679	0.000580	0.000590	
5.2a1	0.000774	0.000811	0.000773	0.000533	0.000531	
5.2a2	0.000854	0.000595	0.000736	0.000647	0.000684	
5.2a3	0.000784	0.000563	0.000678	0.000603	0.000531	
5.2e1	0.000770	0.000692	0.000620	0.000511	0.000649	
5.2e2	0.000802	0.000592	0.000648	0.000703	0.000711	
5.2e3	0.000740	0.000626	0.000637	0.000731	0.000723	
6.1e3	0.000678	0.000712	0.000442	0.000509	0.000561	
6.2e3	0.000769	0.000809	0.000625	0.000777	0.000664	
6.1e2	0.000673	0.000735	0.000640	0.000719	0.000497	
6.2e2	0.000746	0.000625	0.000600	0.000606	0.000622	
6.1e1	0.000631	0.000684	0.000659	0.000756	0.000675	
6.2e1	0.000809	0.000770	0.000684	0.000666	0.000774	
6.1a1	0.000617	0.000629	0.000606	0.000811	0.000578	
6.1a2	0.000631	0.000668	0.000572	0.000836	0.000579	
6.1a3	0.000567	0.000575	0.000671	0.000675	0.000714	
6.2a1	0.000680	0.000583	0.000702	0.000794	0.000669	
6.2a2	0.000650	0.000486	0.000762	0.000615	0.000649	
6.2a3	0.000617	0.000642	0.000660	0.000702	0.000728	
Source of variation	sums of squares (SS)	degrees of freedom (df)	Mean squares (MS)	F-value	P-value	critical F-value
Between group	2.7928E-07	44	6.34727E-09	0.8683252	0.7037724	1.4439497
Within groups	1.31576E-06	180	7.30979E-09			
Total	1.59504E-06	224				
within-sd	8.54973E-05					
effective n	5.00					
s_bb	0					
s_bb_min	1.24139E-05					
u_bb	1.24139E-05					
u_bb(rel.)	1.83570551					

Zn in BAM-M384c

	1	2	3	4	5
1.2e1	0.000214	0.000168	0.000205	0.000168	0.000190
1.2a1	0.000157	0.000161	0.000172	0.000166	0.000173
1.2a2	0.000175	0.000174	0.000224	0.000162	0.000159
1.2a3	0.000189	0.000167	0.000186	0.000159	0.000176
1.2e2	0.000164	0.000160	0.000216	0.000198	0.000178
1.2e3	0.000220	0.000160	0.000179	0.000182	0.000191
2.1a1	0.000212	0.000182	0.000206	0.000211	0.000135
2.1a2	0.000182	0.000188	0.000215	0.000220	0.000158
2.1a3	0.000164	0.000168	0.000215	0.000171	0.000200
3.1e1	0.000171	0.000199	0.000185	0.000172	0.000179
3.2e1	0.000195	0.000155	0.000203	0.000210	0.000189
3.1e2	0.000188	0.000165	0.000194	0.000199	0.000137
3.2e2	0.000217	0.000230	0.000192	0.000193	0.000184
3.1e3	0.000165	0.000173	0.000196	0.000163	0.000129
3.2e3	0.000178	0.000177	0.000199	0.000155	0.000187
4.1e3	0.000189	0.000165	0.000204	0.000178	0.000183
4.1e2	0.000180	0.000193	0.000197	0.000170	0.000172
4.1e1	0.000175	0.000188	0.000188	0.000226	0.000175
4.1a1	0.000191	0.000164	0.000197	0.000191	0.000162
4.1a2	0.000180	0.000195	0.000228	0.000196	0.000181
4.1a3	0.000172	0.000183	0.000219	0.000201	0.000145
4.2a1	0.000172	0.000186	0.000184	0.000170	0.000176
4.2a2	0.000187	0.000184	0.000189	0.000185	0.000141
4.2a3	0.000177	0.000176	0.000195	0.000157	0.000183
5.1a1	0.000194	0.000173	0.000211	0.000179	0.000150
5.1a2	0.000190	0.000228	0.000188	0.000205	0.000162
5.1a3	0.000174	0.000161	0.000190	0.000176	0.000174
5.2a1	0.000150	0.000204	0.000200	0.000188	0.000132
5.2a2	0.000182	0.000193	0.000204	0.000154	0.000228
5.2a3	0.000169	0.000173	0.000204	0.000187	0.000167
5.2e1	0.000200	0.000155	0.000237	0.000217	0.000142
5.2e2	0.000164	0.000160	0.000181	0.000151	0.000148
5.2e3	0.000188	0.000168	0.000182	0.000162	0.000120
6.1e3	0.000165	0.000232	0.000203	0.000168	0.000149
6.2e3	0.000173	0.000167	0.000216	0.000204	0.000204
6.1e2	0.000179	0.000175	0.000224	0.000171	0.000187
6.2e2	0.000160	0.000191	0.000204	0.000196	0.000154
6.1e1	0.000217	0.000169	0.000217	0.000181	0.000182
6.2e1	0.000182	0.000171	0.000198	0.000174	0.000173
6.1a1	0.000141	0.000194	0.000158	0.000198	0.000195
6.1a2	0.000185	0.000176	0.000212	0.000209	0.000139
6.1a3	0.000180	0.000180	0.000198	0.000196	0.000151
6.2a1	0.000219	0.000174	0.000214	0.000220	0.000189
6.2a2	0.000178	0.000156	0.000207	0.000193	0.000151
6.2a3	0.000164	0.000194	0.000185	0.000180	0.000170

Source of variation	sums of squares (SS)	degrees of freedom (df)	Mean squares (MS)	F-value	P-value	critical F-value
Between group	1.85458E-08	44	4.21496E-10	0.8649233	0.7092728	1.4439497
Within groups	8.7718E-08	180	4.87322E-10			
Total	1.06264E-07	224				
within-sd	2.20754E-05					
effective n	5.00					
s_bb	0					
s_bb_min	3.20525E-06					
u_bb	3.20525E-06					
u_bb(rel.)	1.754445083					

**Annex 2:** Calculation of uncertainty contribution of potential inhomogeneity (area) ( $u_{bb}(rel.)$  here means  $u_{bb}$  (rel) Area in Table 39), data from BAM-M384c

Ag in BAM-M384c:

r_0	0.001386143	0.001431857											
r_in	0.001405	0.001407	0.00142	0.001433	0.001408	0.001404							
r_out	0.001388	0.001389	0.001417	0.001429	0.001461	0.001418	0.001424	0.001436	0.001422	0.001427	0.00141	0.00143	
<i>Source of variation</i>	<i>sums of squares (SS)</i>	<i>degrees of freedom (df)</i>	<i>Mean squares (MS)</i>	<i>F-value</i>	<i>P-value</i>	<i>critical F-value</i>							
Between groups	4.1445E-10	2	2.07225E-10	0.589630077	0.565481098	3.591530568							
Within groups	5.97464E-09	17	3.51449E-10										
Total	6.38909E-09	19											
within-sd	1.8747E-05												
effective n	5.40												
s_bb	0												
s_bb_min	4.72476E-06												
u_bb	4.72476E-06												
u_bb(rel.)	0.333363357												

Bi in BAM-M384c:

r_0	0.000338263	0.000425737											
r_in	0.000389	0.0004	0.000387	0.000357	0.000432	0.000386							
r_out	0.000386	0.000381	0.00036	0.000414	0.000398	0.00042	0.000409	0.00036	0.000409	0.000388	0.000398	0.00039	
<i>Source of variation</i>	<i>sums of squares (SS)</i>	<i>degrees of freedom (df)</i>	<i>Mean squares (MS)</i>	<i>F-value</i>	<i>P-value</i>	<i>critical F-value</i>							
Between groups	1.99717E-10	2	9.98583E-11	0.155444538	0.857237491	3.591530568							
Within groups	1.09209E-08	17	6.42405E-10										
Total	1.11206E-08	19											
within-sd	2.53457E-05												
effective n	5.40												
s_bb	0												
s_bb_min	6.38782E-06												
u_bb	6.38782E-06												
u_bb(rel.)	1.632044478												

Cd in BAM-M384c:

r_0	0.000392863	0.000473137											
r_in	0.000449	0.00048	0.00043	0.00042	0.000432	0.00043							
r_out	0.000425	0.000386	0.000412	0.000431	0.000443	0.000412	0.000422	0.00041	0.000445	0.000477	0.000401	0.000456	
Source of variation	sums of squares (SS)	degrees of freedom (df)	Mean squares (MS)	F-value	P-value	critical F-value							
Between groups	7.3505E-10	2	3.67525E-10	0.494789783	0.618211695	3.591530568							
Within groups	1.26274E-08	17	7.4279E-10										
Total	1.33625E-08	19											
within-sd	2.72542E-05												
effective n	5.40												
s_bb	0												
s_bb_min	6.86881E-06												
u_bb	6.86881E-06												
u_bb(rel.)	1.592398162												

Co in BAM-M384c:

r_0	0.00032449	0.00034551											
r_in	0.000345	0.000349	0.000346	0.000338	0.000333	0.000345							
r_out	0.000347	0.000339	0.000347	0.000341	0.000348	0.000346	0.000344	0.000344	0.000346	0.00034	0.000351	0.000345	
Source of variation	sums of squares (SS)	degrees of freedom (df)	Mean squares (MS)	F-value	P-value	critical F-value							
Between groups	1.682E-10	2	8.41E-11	2.687906157	0.096760018	3.591530568							
Within groups	5.31901E-10	17	3.12883E-11										
Total	7.00101E-10	19											
within-sd	5.59359E-06												
effective n	5.40												
s_bb	3.12729E-06												
s_bb_min	1.40974E-06												
u_bb	3.12729E-06												
u_bb(rel.)	0.91121516												



Cr in BAM-M384c:

r_0	0.001020548	0.001403452											
r_in	0.001342	0.001223	0.001171	0.001134	0.001106	0.001027							
r_out	0.001134	0.001134	0.001151	0.001156	0.001282	0.001092	0.001079	0.0012	0.001079	0.001052	0.001051	0.001027	
Source of variation	sums of squares (SS)	degrees of freedom (df)	Mean squares (MS)	F-value	P-value	critical F-value							
Between groups	1.95121E-08	2	9.75606E-09	0.877684857	0.433758482	3.591530568							
Within groups	1.88966E-07	17	1.11157E-08										
Total	2.08479E-07	19											
within-sd	0.000105431												
effective n	5.40												
s_bb	0												
s_bb_min	2.65715E-05												
u_bb	2.65715E-05												
u_bb(rel.)	2.324310073												

Fe in BAM-M384c:

r_0	0.003544624	0.003645376											
r_in	0.003659	0.00364	0.003636	0.003645	0.003691	0.0037							
r_out	0.003599	0.003616	0.003675	0.003625	0.003573	0.003639	0.003616	0.003661	0.003595	0.003659	0.003633	0.003629	
Source of variation	sums of squares (SS)	degrees of freedom (df)	Mean squares (MS)	F-value	P-value	critical F-value							
Between groups	8.33545E-09	2	4.16772E-09	3.839152197	0.042085805	3.591530568							
Within groups	1.84549E-08	17	1.08558E-09										
Total	2.67904E-08	19											
within-sd	3.29482E-05												
effective n	5.40												
s_bb	2.38907E-05												
s_bb_min	8.30386E-06												
u_bb	2.38907E-05												
u_bb(rel.)	0.657413203												

Mg in BAM-M384c:

r_0	0.000288477	0.000305523											
r_in	0.000308	0.000315	0.000312	0.000307	0.000304	0.000311							
r_out	0.000301	0.000313	0.000323	0.000324	0.000316	0.000309	0.000299	0.000296	0.000306	0.000307	0.000305	0.000313	
<i>Source of variation</i>	<i>sums of squares (SS)</i>	<i>degrees of freedom (df)</i>	<i>Mean squares (MS)</i>	<i>F-value</i>	<i>P-value</i>	<i>critical F-value</i>							
Between groups	2.76383E-10	2	1.38192E-10	2.164318418	0.14542179	3.591530568							
Within groups	1.08545E-09	17	6.385E-11										
Total	1.36183E-09	19											
within-sd	7.99062E-06												
effective n	5.40												
s_bb	3.71039E-06												
s_bb_min	2.01386E-06												
u_bb	3.71039E-06												
u_bb(rel.)	1.204085098												

Mn in BAM-M384c:

r_0	0.000786	0.00091											
r_in	0.000924	0.000891	0.000927	0.000875	0.00086	0.000846							
r_out	0.000907	0.000872	0.000875	0.000874	0.000959	0.000845	0.000884	0.000876	0.000817	0.000851	0.000814	0.000843	
<i>Source of variation</i>	<i>sums of squares (SS)</i>	<i>degrees of freedom (df)</i>	<i>Mean squares (MS)</i>	<i>F-value</i>	<i>P-value</i>	<i>critical F-value</i>							
Between groups	2.71545E-09	2	1.35772E-09	0.759010956	0.48335007	3.591530568							
Within groups	3.04097E-08	17	1.78881E-09										
Total	3.31252E-08	19											
within-sd	4.22943E-05												
effective n	5.40												
s_bb	0												
s_bb_min	1.06593E-05												
u_bb	1.06593E-05												
u_bb(rel.)	1.222681691												

Ni in BAM-M384c:

r_0	5.40	5.88				
r_in	5.76	5.71	5.80	5.67		
r_out	5.83	5.90	6.78	5.86		
Source of variation	sums of squares (SS)	degrees of freedom (df)	Mean squares (MS)	F-value	P-value	critical F-value
Between groups	0.3732701	2	0.18663505	1.729778037	0.245214844	4.737414128
Within groups	0.755267625	7	0.107895375			
Total	1.128537725	9				
within-sd	0.328474314					
effective n	3.20					
s_bb	0.156863471					
s_bb_min	0.134248491					
u_bb	0.156863471					
u_bb(rel.)	2.676759679					

Pb in BAM-M384c:

r_0	0.000842753	0.000963247											
r_in	0.000942	0.001015	0.000943	0.001	0.001001	0.000977							
r_out	0.001005	0.000926	0.001008	0.000998	0.000942	0.001029	0.001006	0.000949	0.000911	0.000935	0.000898	0.000894	
Source of variation	sums of squares (SS)	degrees of freedom (df)	Mean squares (MS)	F-value	P-value	critical F-value							
Between groups	8.8375E-09	2	4.41875E-09	1.998172366	0.166185997	3.591530568							
Within groups	3.75937E-08	17	2.2114E-09										
Total	4.64312E-08	19											
within-sd	4.70255E-05												
effective n	5.26												
s_bb	2.04792E-05												
s_bb_min	1.20048E-05												
u_bb	2.04792E-05												
u_bb(rel.)	2.134917048												

S in BAM-M384c:

r_0	0.000298946	0.000405054										
r_in	0.000344	0.000405	0.000357	0.000338	0.000328	0.00034						
r_out	0.000373	0.000389	0.000367	0.00033	0.000353	0.000341	0.000287	0.000389	0.000311	0.00037	0.000293	0.000279
Source of variation	sums of squares (SS)	degrees of freedom (df)	Mean squares (MS)	F-value	P-value	critical F-value						
Between groups	6.72133E-10	2	3.36067E-10	0.21307188	0.810223519	3.591530568						
Within groups	2.68132E-08	17	1.57725E-09									
Total	2.74853E-08	19										
within-sd	3.97146E-05											
effective n	5.40											
s_bb	0											
s_bb_min	1.00092E-05											
u_bb	1.00092E-05											
u_bb(rel.)	2.902049693											

Sb in BAM-M384c:

r_0	0.00081537	0.00103063										
r_in	0.000931	0.000903	0.000848	0.000796	0.000955	0.000861						
r_out	0.000958	0.001012	0.000981	0.000971	0.000925	0.00097	0.000993	0.000928	0.000959	0.000795	0.000848	0.00096
Source of variation	sums of squares (SS)	degrees of freedom (df)	Mean squares (MS)	F-value	P-value	critical F-value						
Between groups	1.4084E-08	2	7.042E-09	1.446233397	0.263004014	3.591530568						
Within groups	8.27764E-08	17	4.8692E-09									
Total	9.68604E-08	19										
within-sd	6.97797E-05											
effective n	5.40											
s_bb	2.00592E-05											
s_bb_min	1.75864E-05											
u_bb	2.00592E-05											
u_bb(rel.)	2.175615036											

Te in BAM-M384c:

r_0	0.000650732	0.001035268										
r_in	0.000837	0.000691	0.000792	0.000564	0.000822	0.000837						
r_out	0.00079	0.000693	0.000819	0.000829	0.000844	0.000802	0.000775	0.000723	0.000668	0.000777	0.000755	0.000625
Source of variation	sums of squares (SS)	degrees of freedom (df)	Mean squares (MS)	F-value	P-value	critical F-value						
Between groups	1.30275E-08	2	6.51372E-09	0.599195447	0.560448128	3.591530568						
Within groups	1.84803E-07	17	1.08708E-08									
Total	1.97831E-07	19										
within-sd	0.000104263											
effective n	5.40											
s_bb	0											
s_bb_min	2.62772E-05											
u_bb	2.62772E-05											
u_bb(rel.)	3.428427874											

Zn in BAM-M384c:

r_0	0.000144328	0.000219672										
r_in	0.000208	0.000202	0.00018	0.000169	0.00015	0.00018						
r_out	0.000179	0.000185	0.000163	0.000187	0.000176	0.000181	0.000151	0.000169	0.000166	0.000157	0.000154	0.000156
Source of variation	sums of squares (SS)	degrees of freedom (df)	Mean squares (MS)	F-value	P-value	critical F-value						
Between groups	8.06383E-10	2	4.03192E-10	0.994442372	0.390454502	3.591530568						
Within groups	6.89256E-09	17	4.05445E-10									
Total	7.69895E-09	19										
within-sd	2.01357E-05											
effective n	5.40											
s_bb	0											
s_bb_min	5.07475E-06											
u_bb	5.07475E-06											
u_bb(rel.)	2.919037384											